


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	Thiruvananthapuram
2	Name of Hospital	FHC Kanjiramkulam.
3	Name of Equipment with Make, Model and Serial Number	Baby weighing machine (analogue) MISAKI
4	Equipment ID & Barcode	210268 0144529.
5	Date of purchase / Year of manufacture / Installation Date	21.05.2014.
6	Warranty details (Yes/No)	No
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/ CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	12.11.2023.
9	Action taken	Try to service
10	Present status of the equipment (Fully damaged / partially damaged)	Slightly damaged
11	Recommendations for repair (required service details)	Checked the equipment. Found equipment in suited condition and weighing mechanism complete
12	Cost of spares (specify parts and cost)	NA.

13	Asset Value	1300/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	No
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Attached
16	Reasons for recommending the equipment as BER	Checked the equipment. Found equipment is rusted condition and weighing mechanism complete so it not serviceable so recommending the equipment as BER
17	Name & Signature of CYRIX Authority	


*Not mandatory #Based on the period of life and value as per the BER guidelines

* **Attach Photograph**


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Equipment fully rusted - so not serviceable.
so RBER.

MANESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


6.12.2023
Signature of JC BM (NHM)

Date 01/12/2023




Signature of Superintendent / Medical Officer (i/c)



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : **154502**

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>Family Health Center</u></p> <p>Address <u>Kojarankulam, Thiruvananthapuram</u></p> <p>Ph : <u>9074338992</u></p>	<p>Call Registration Date : <u>18.11.2023</u></p> <p>Caller ID : <u>21026</u></p> <p>Date of Visit : <u>24.11.2023</u></p> <p>Asset No. : <u>0144529</u></p> <p>EQPT Name : <u>weighing machine (Baby-weight)</u></p> <p>Manufacture <u>Misaki</u> Model : <u>NA</u></p> <p>S. No. <u>NA</u> Dept. <u>FWC Karichal</u></p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Rusted condition, weighing mechanism complaint

Action Taken : checked the equipment found equipment is rusted condition & weighing mechanism complaint. So it's not serviceable

Completed Date : 24.11.2023 Time : 1:00pm Spare Required



Spare Replaced Requested


Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrux Engineer	Date	Start Time	End Time
<u>Mohammed Sherif</u>	<u>24.11.2023</u>	<u>11:00pm</u>	<u>1:00pm</u>

Customer Remark Completed Pending

<p>Service Engineer Name : <u>Mohammed Sherif</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>24.11.2023</u></p> <p>Contact Number : <u>7994042445</u></p>	<p>Customer Name : <u>[Signature]</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>[Signature]</u></p> <p>Contact Number : <u>9074338992</u></p> <p>Designation : <u>Naming Officer and</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
---	--

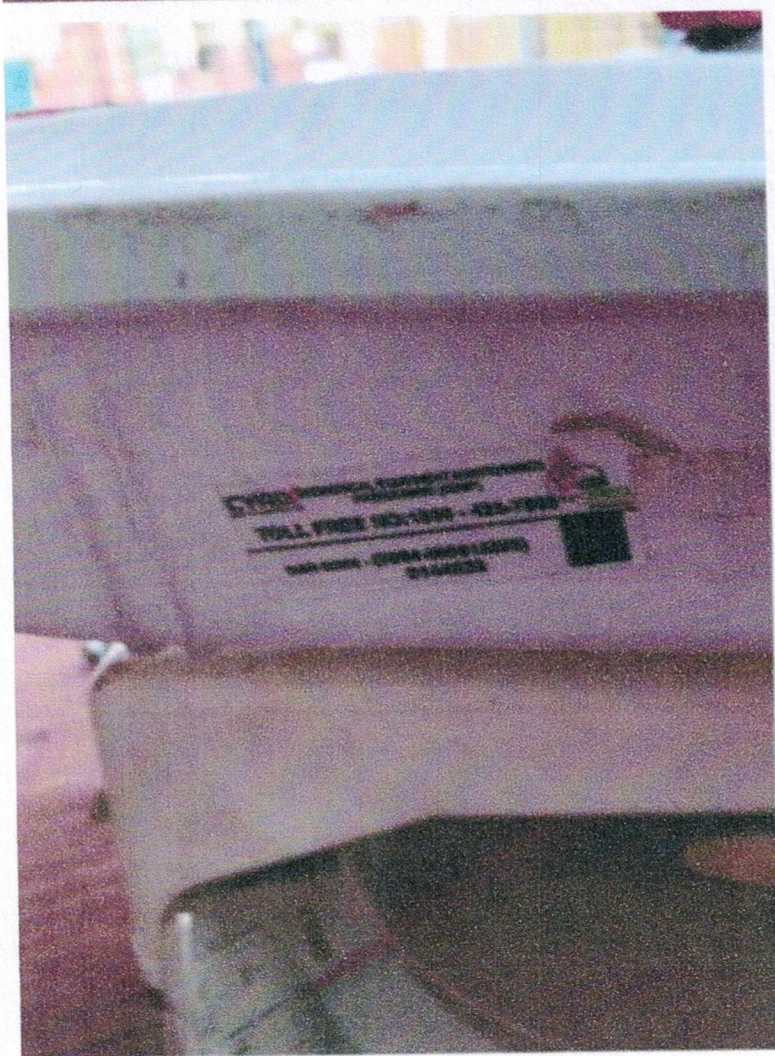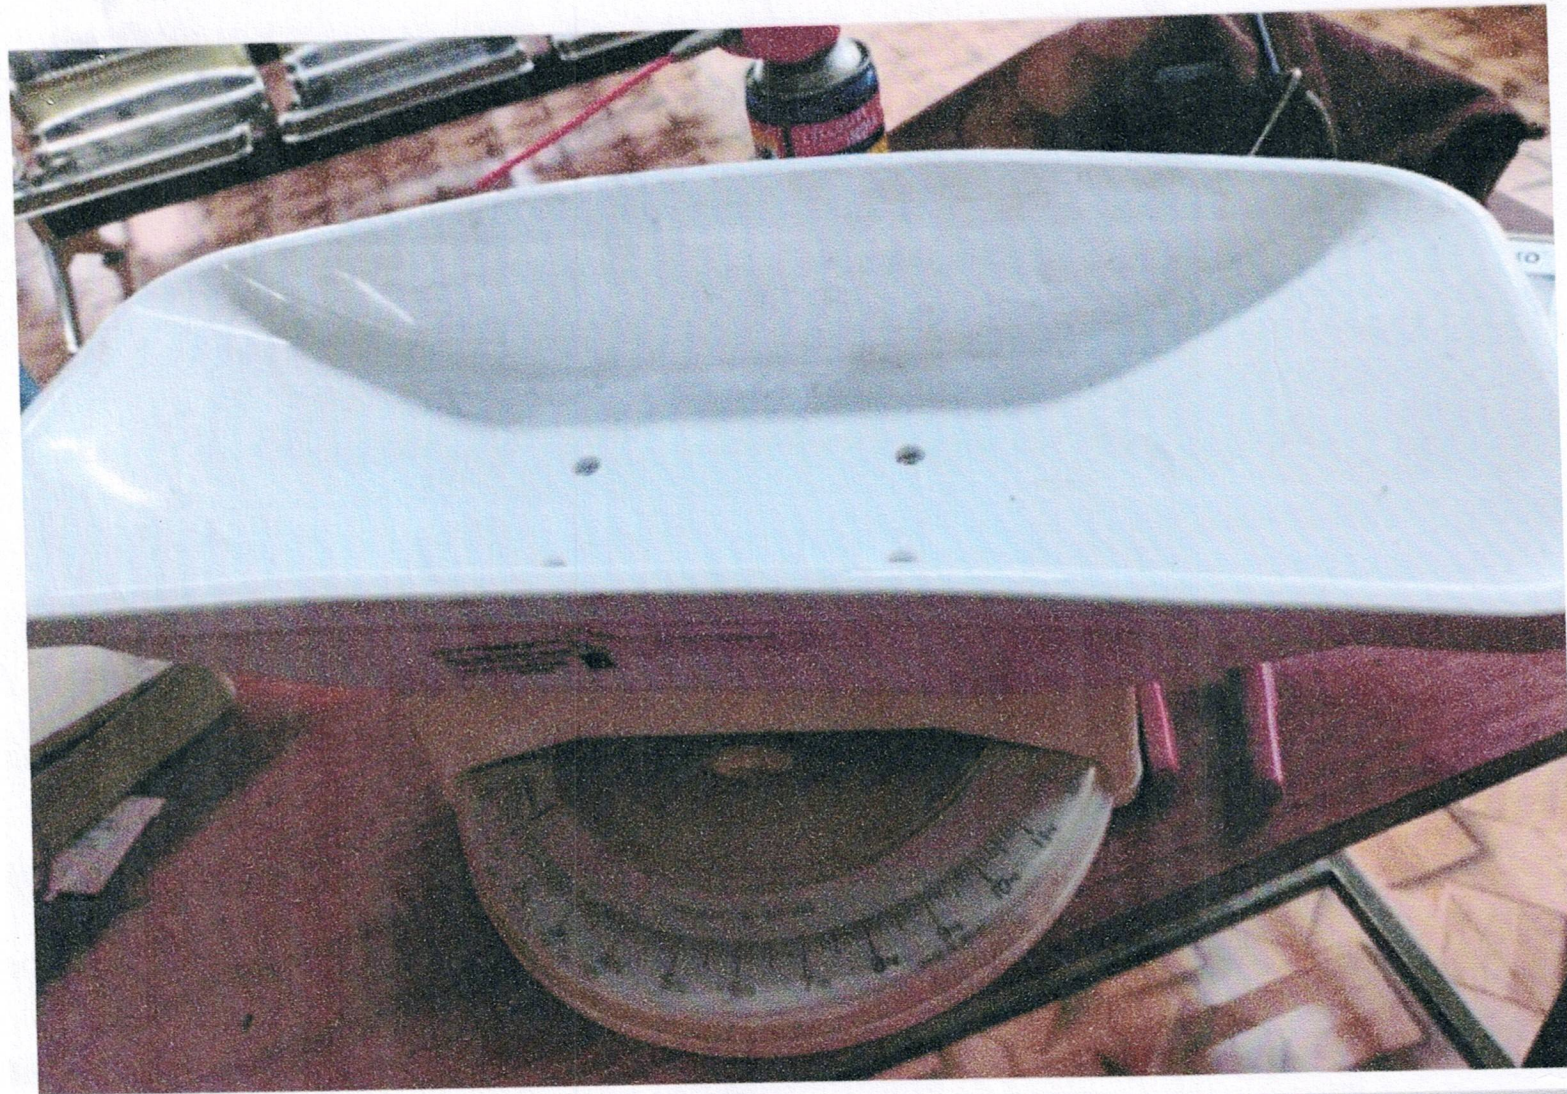

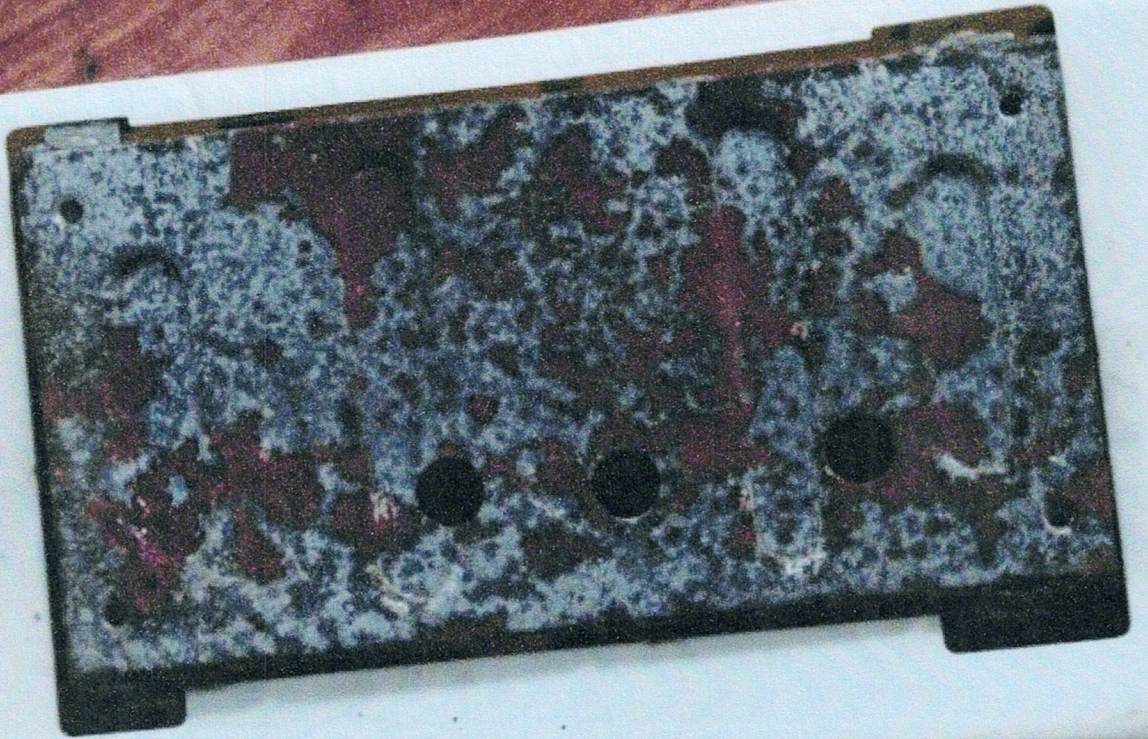

Elaby Scale
MISUMI

MADE IN JAPAN