



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : **161337**

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>FHC-KUNNAMANGALAM</u></p> <p>Address <u>KOZHIKODE</u> <u>KERALA</u></p> <p>Ph : <u>9539159020</u></p>	<p>Call Registration Date : <u>08/01/2024</u></p> <p>Caller ID : <u>89548</u></p> <p>Date of Visit : <u>09/01/2024</u></p> <p>Asset No. : <u>1143182</u></p> <p>EQPT Name : <u>NEBULISER</u></p> <p>Manufacture <u>LIFECARE</u> Model : <u>CX1-03</u></p> <p>S. No. <u>082019</u> Dept. <u>OP</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : FUMES NOT GETTING

Action Taken : CHECKED AND FOUND COMPRESSOR MOTOR WITH PISTON DEFECTIVE. NEED TO REPLACE THESE SPARES FOR FURTHER CHECKING WORKING CONDITION OF THESE EQUIPMENT.

Completed Date : 15/01/24 Time : 3.00 P.M. Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.	-----			
2.	-----			
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>PRABHATH.K</u>	<u>15/01/24</u>	<u>2.30 PM</u>	<u>3.00 PM</u>

Customer Remark Completed Pending

Fumes not getting old machine since 20/9/2017.


<p>Service Engineer Name : <u>PRABHATH.K</u></p> <p>Signature </p> <p>Date : <u>15/01/24</u></p> <p>Contact Number : <u>4593847126</u></p>	<p>Customer Name : <u>Dr. Abdur Jaleel</u></p> <p>Signature </p> <p>Date : <u>15/01/24</u></p> <p>Contact Number : <u>9539159020</u></p> <p>Designation : <u>Medical Officer</u></p> <p>Hospital Seal : </p>
--	--

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KOZHIKODE
2	Name of Hospital	PHC KUNNAMANGALAM
3	Name of Equipment with Make, Model and Serial Number	Equipment : Nebuliser Make : Lifecare Model :CN-03 SN : NA
4	Equipment ID & Barcode	89548 & 1143182
5	Date of purchase / Year of manufacture /Installation Date	20-09-2017
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	08-01-2024 (Toll free)
9	Action taken	Regarding the inspection of the equipment found that Compressor motor with piston defective.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	NA


13	Asset Value	Rs . 1353/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found Compressor motor with piston defective. Equipment installed on 20-09-2017 and covered upto 6+ years. Quotation not submitted since spares are not available in the market .So recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	PRABHATH.K 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Checked & found that compressors motor with piston are defective. Tubing connects is also defective. Equipment installed on 20/09/2017. Spares are not available in the market. So recommended for condemnation.

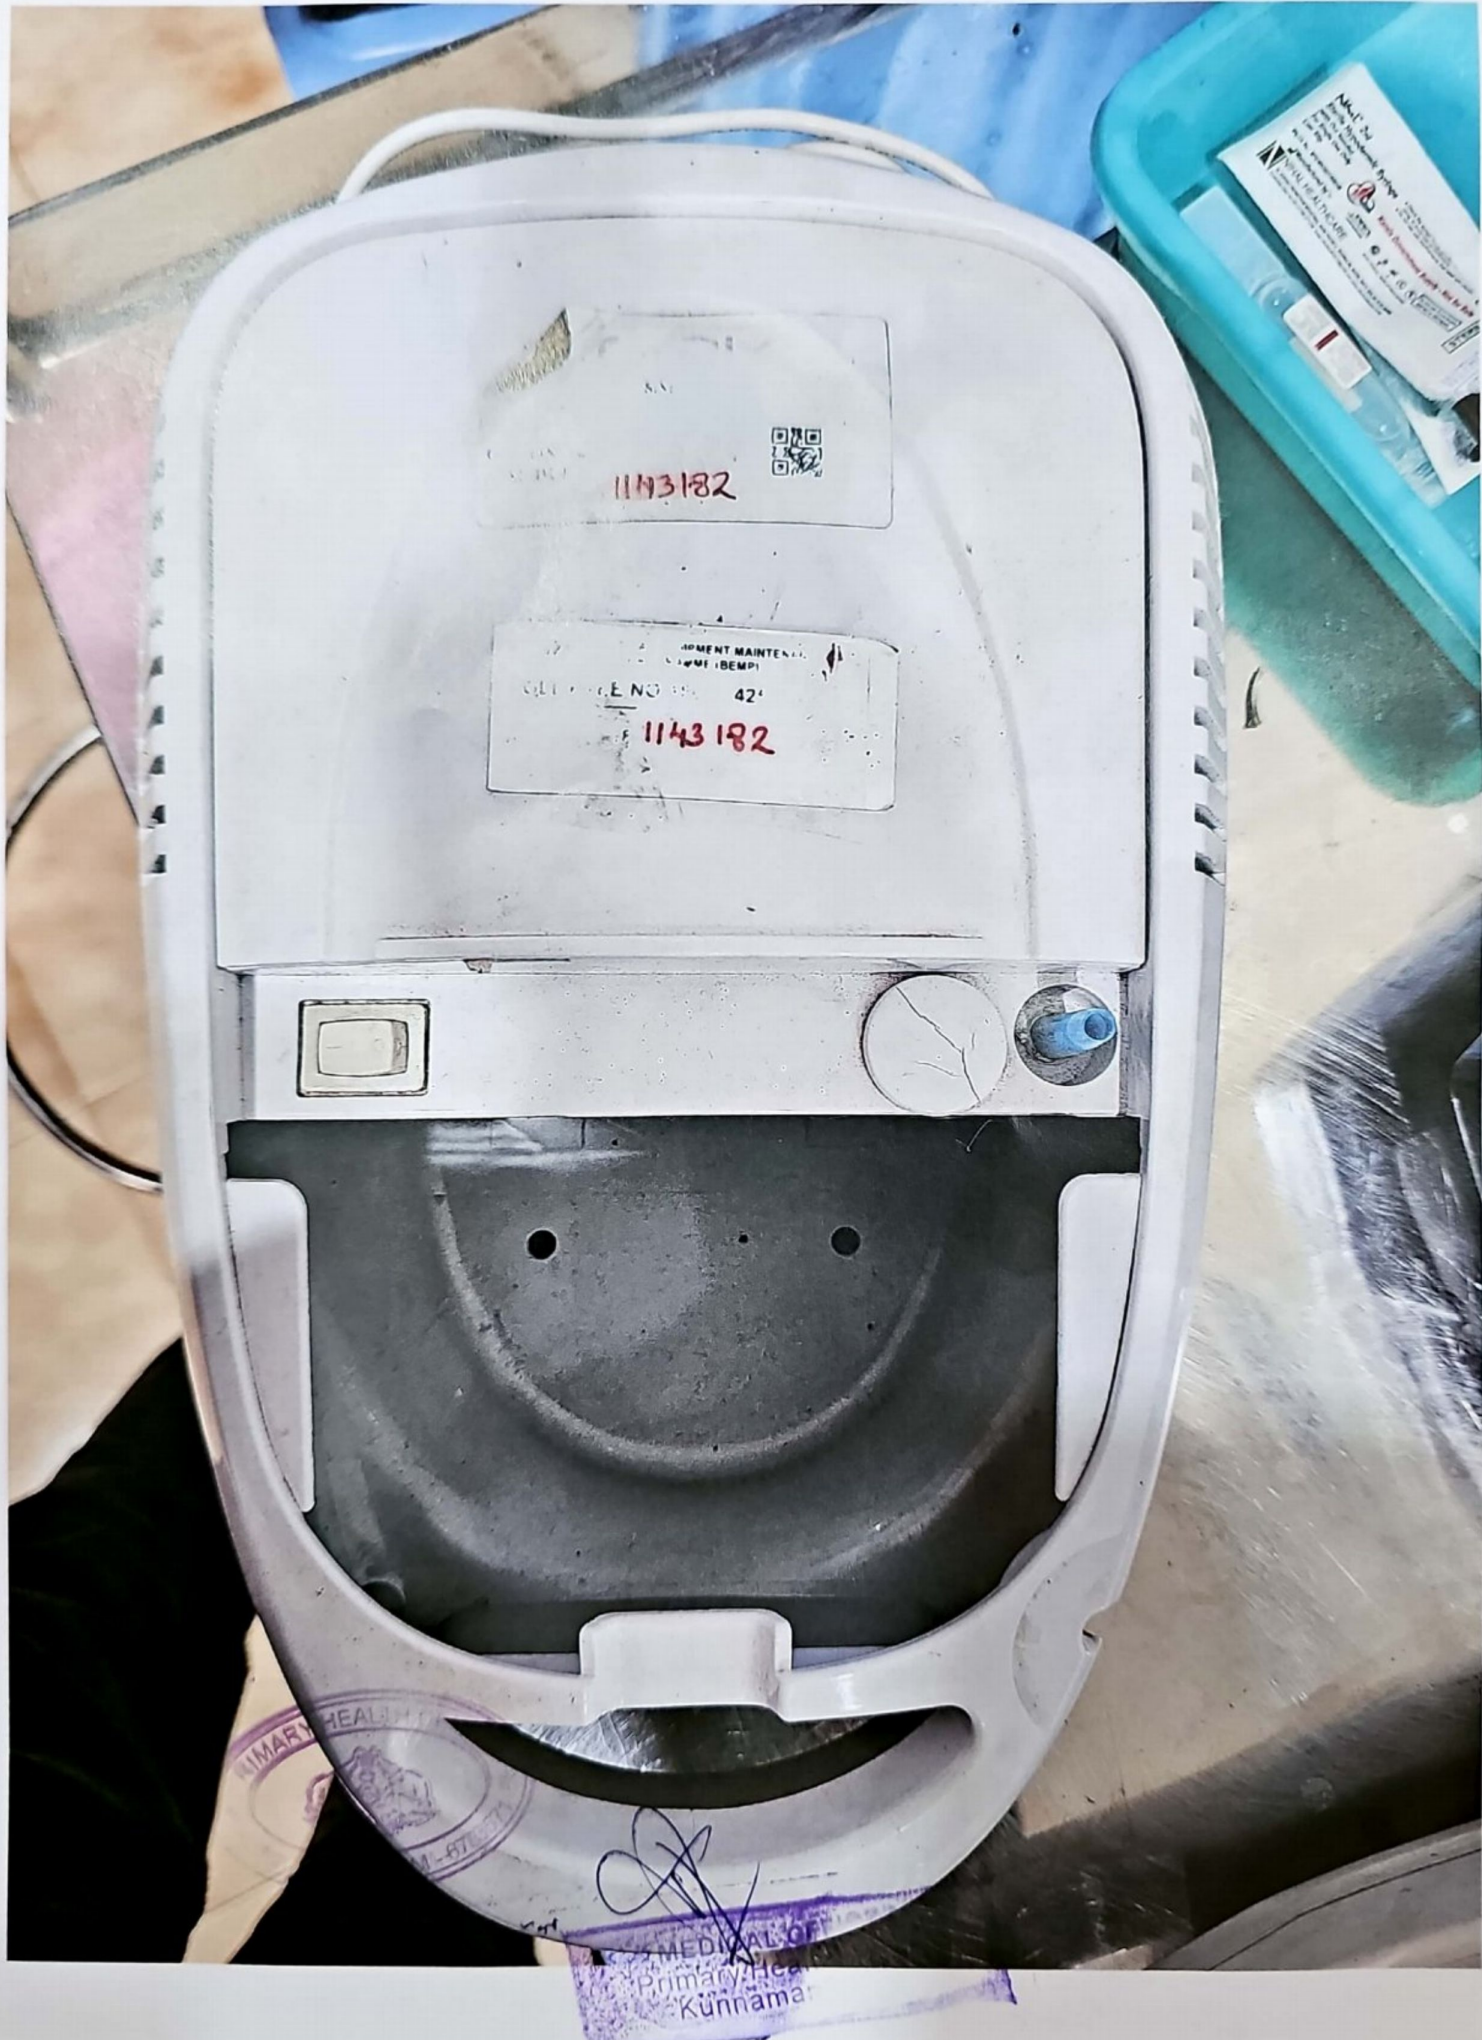

 Consultant Bio Medicine, Signature of JC BM (NHM)
 National Health Mission
 Kozhikode

Date _____

Mechine is not working, (old vers 2017)


 Signature of 1.24
 Superintendent Medical Officer (C)
 MEDICAL OFFICER
 Primary Health Centre
 Kunnamangalam


 PRIMARY HEALTH CENTRE
 KUNNAMANGALAM - 673571





300721UG
X12h)

2815H11

Compressor Nebulizer
Model : CN-03
Input : 230V / 50 Hz
Power : 80 VA
Lot No : 082019
Mfg Date : Aug 2019
Shelf Life : Not Applicable
Made in India

for
MEDICAL OFFICER
Primary Health Centre
Kunnamangalam