


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

418


PROFORMA

Sl. No	Particulars	Details
1	Name of District	Tiruvananthapuram
2	Name of Hospital	THQH Chirayinkeezh
3	Name of Equipment with Make, Model and Serial Number	Anesthesia Machine CG Datex Ohmeda Aspire 7100 SN: AM X132900243WA
4	Equipment ID & Barcode	84408 & 0121473
5	Date of purchase / Year of manufacture / Installation Date	2-5-2014
6	Warranty details (Yes/No)	No
7	*AMC/ CAMC Period agreed at the time of purchase	N/A
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	7-12-2023
9	Action taken	Switch pressure and PCA Vest Monitoring board complaint.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged.
11	Recommendations for repair (required service details)	Switch pressure and PCA Vest monitoring board complaint. This model was discontinued, spare parts are not available to repair.
12	Cost of spares (specify parts and cost)	NA



BIOMEDICAL EQUIPMENT

CHIRAYINKEEZH


13	Asset Value	8,63,763
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Attached Cyrix Service Report - OEM letter
16	Reasons for recommending the equipment as BER	Switch pressure and PCA Vest monitoring board compliant model as per per the EOL letter from the OEM. It is recommended for RBER
17	Name & Signature of CYRIX Authority	Kochu Prakash VS 

*Not mandatory **#Based on the period of life and value as per the BER guidelines**


* **Attach Photograph**

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:
 Model is discontinued. So can be RBER as per tender norms (late submission)


MANEESHA MOHAN M.R.
 Junior Consultant (Biomedical)
 National Health Mission
 Thiruvananthapuram


 15-1-2024
 Signature of JC BM (NHM)

Date 8/1/24



Seal


 Signature of
 Superintendent / Medical Officer (i/c)

SUPERINTENDENT
 Thaluk Head Quarters Hospital
 Chirayinkeezhu



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 172661

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

418

<p>Health Facility : <u>THQU</u></p> <p>Address : <u>Chirayinkeezh</u> <u>Thiruvananthapuram</u></p> <p>Ph : <u>9995227140</u></p>	<p>Call Registration Date : <u>7.12.2023</u></p> <p>Caller ID : <u>84408</u></p> <p>Date of Visit : <u>9.12.2023</u></p> <p>Asset No. : <u>0121473</u></p> <p>EQPT Name : <u>Anesthesia Machine</u></p> <p>Manufacture : <u>Ge</u> Model : <u>Ohmeda</u></p> <p>S. No. <u>AMX.13290023</u> Dept. : <u>OT</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : Checked and found that switch pressure and PCA Med Monitoring board complaints.
This model was discontinued and spare parts not available to repair.

Completed Date : Time : Spare Required



Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Keshu Prakash-V8</u>			

Customer Remark Completed Pending

<p>Service Engineer Name : <u>Keshu Prakash-V8</u></p> <p>Signature : </p> <p>Date : _____</p> <p>Contact Number : <u>9072522086</u></p>	<p>Customer Name : <u>Koi</u></p> <p>Signature : </p> <p>Date : _____</p> <p>Contact Number : <u>999522</u></p> <p>Designation : <u>Bio medical Engineer</u></p> <p>Hospital Seal : </p>
--	--

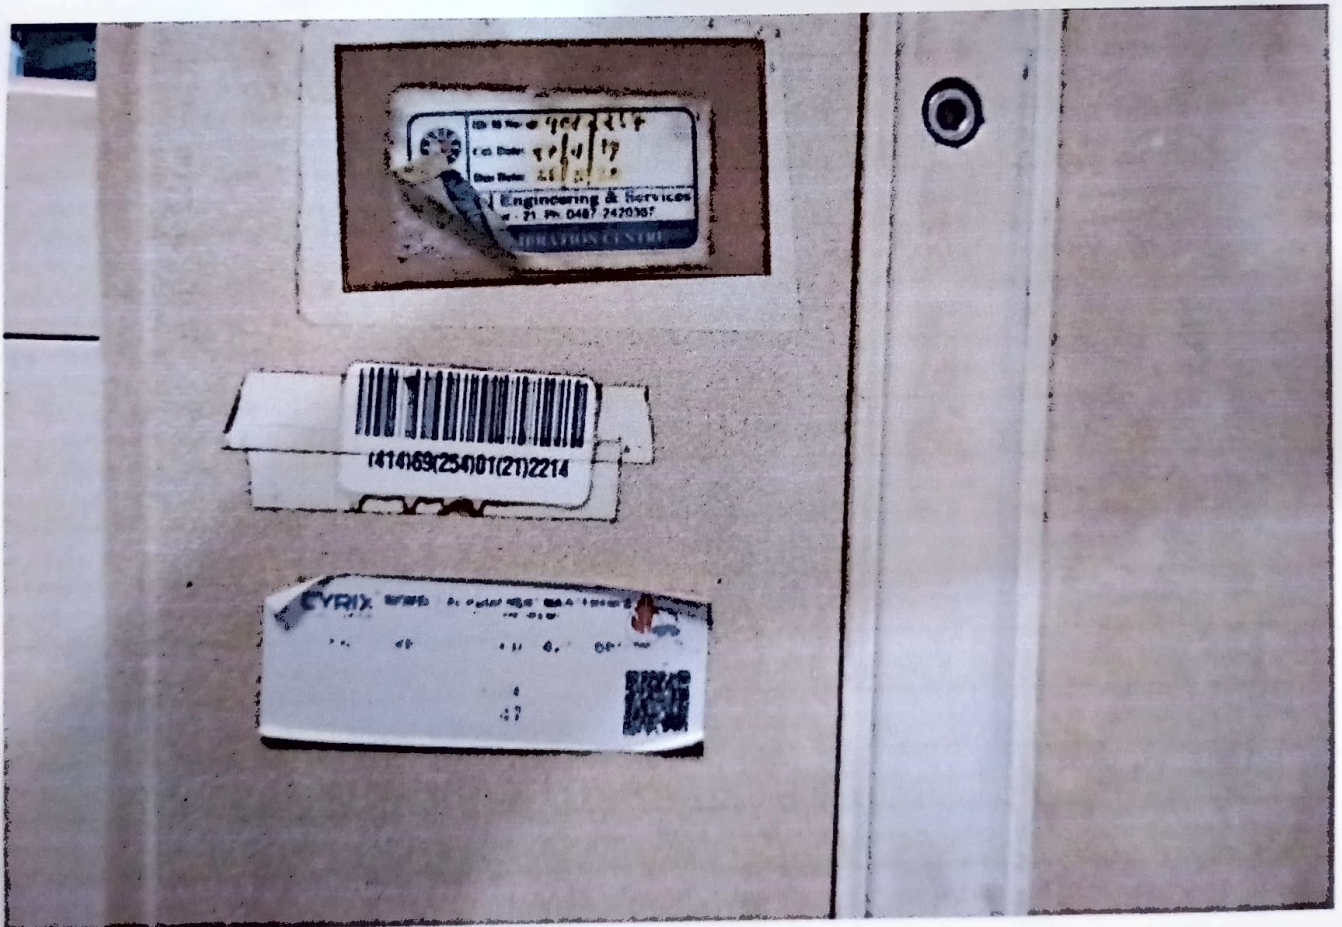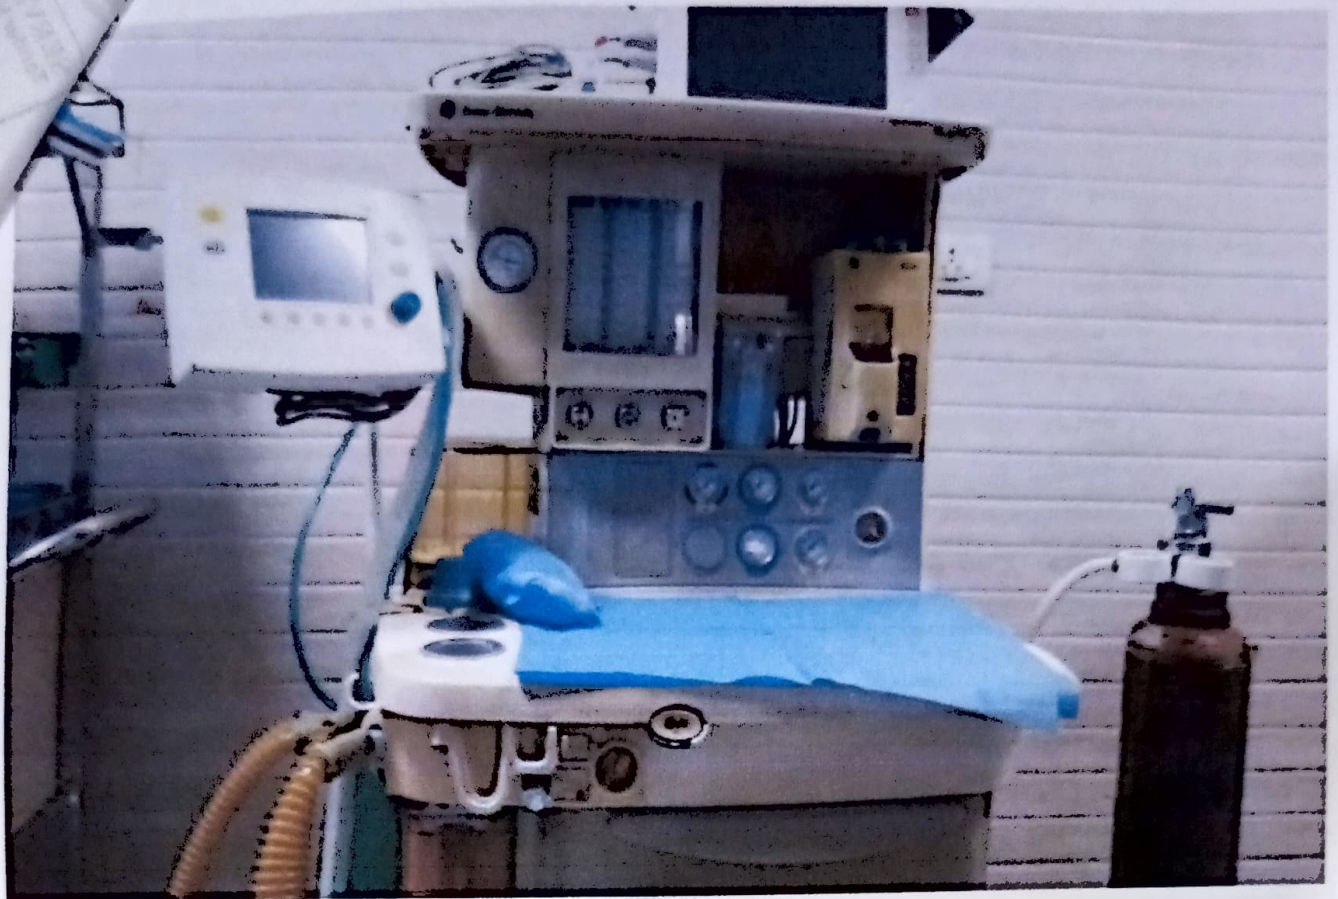

**WIPRO GE HEALTHCARE**

CIN: U33111KA1990PTC016063
No. 4 Kadugodi Industrial Area,
Bangalore 560067, Karnataka
India, T: 91 80 4180 1000
F 91 80 4180 1290
website: www.gehealthcare.in

Letter No: 2022/EOGS/LCS/ANESTHESIA/AESPIRE/567

Date: 27 Sep 2022

To,
1557613
TRIVANDRUM
, CHIRAYINKEEZHU,
CHIRAYINKEEZHU, Kerala - 695304

SUBJECT: IMPORTANT END OF SERVICE SUPPORT NOTIFICATION FOR: AESPIRE 100/7100/7900

Dear Customer,

We know it is important to your planning to have advanced notice of changes in the status of your maturing medical equipment. That's why we take a proactive approach to notify you when our products will reach an **End of Service Support (EOSS)** status.

Our records indicate that your facility has the following equipment that will reach its EOSS status as of the date indicated in the table below. After the given EOSS date, GE Healthcare will (1) no longer offer full-service support or contracts with parts or uptime guarantees and (2) remove these products from your service contract or transition to an "End of Service Support" coverage. Until the EOSS date, GE Healthcare will continue to deliver to our service commitments.

Asset	Equipment Description	EOSS Date
LCS_S_1009-9000-000_AMX13290273WA	S/5 AESPIRE CONFIG	31 st May 2023

Although many factors are considered when determining that a product has reached EOSS status, the main reason for this decision is the lack of availability of parts required for maintenance and repair. As equipment ages and technology advances, outside suppliers cease to produce many of the parts and components utilized in older systems. As a result, GE Healthcare is unable to procure certain necessary replacement parts to service these products.

We understand the potential impact that this notification may cause you and our goal is to help you find the best solution to address your needs. Your GE Healthcare team will contact you to discuss technology replacement opportunities and service options available after the EOSS date.

Sincerely,

Naresh Pradhan
Manager - Service Operations
WIPRO GE HEALTHCARE PVT. LTD.