



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 175373

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <u>W&C Hospital</u>	Call Registration Date : <u>05/01/2024</u>
Address <u>Palakkad</u>	Caller ID : <u>88969</u>
Ph : <u>9495170195</u>	Date of Visit : <u>06/01/2024</u>
	Asset No. : <u>0912440</u>
	EQPT Name : <u>Digital BP Apparatus</u>
	Manufacture <u>CITIZEN</u> Model : <u>CH-432</u>
	S. No. <u>NA</u> Dept. <u>Antenatal ward</u>

Service Classification : Breakdown Call **PMS** **Calibration** **Cust.Training**

Problem Identified : Error 4, Display issues

Action Taken : checked and found that display, main board, pump and digital BP cuff are faulty. For further checking need to replace main board, display, pump & digital BP cuff.

Completed **Date :** 10/01/24 **Time :** 11:00am **Spare Required**

Spare Replaced **Requested**

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>LIBIL LAL-L</u>	<u>10/01/24</u>	<u>10:00AM</u>	<u>11:00AM</u>

Customer Remark **Completed** **Pending**



Service Engineer Name : LIBIL LAL-L
Signature : [Signature]
Date : 10/01/2024
Contact Number : 8891382686

Customer Name : REENA. C-S
Signature : [Signature]
Date : 10/1/25
Contact Number : 9495170195
Designation : SNO.
Hospital Seal :


SUPERINTENDENT
Govt. W&C Hospital
Palakkad

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	PALAKKAD
2	Name of Hospital	W&C Hospital Palakkad
3	Name of Equipment with Make, Model and Serial Number	Digital BP Apparatus Make : CITIZEN Model : CH-432 SN : NA
4	Equipment ID & Barcode	88969 / 0912440
5	Date of purchase / Year of manufacture / Installation Date	26/10/2016
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	05/01/2024 (Toll free)
9	Action taken	Checked & found main board display, cuff and pump faulty. For further checking enquired for spare
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Need to replace * main board * Display * Pump * Digital BP cuff
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	2200/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX service report attached
16	Reasons for recommending the equipment as BER	Checked equipment found BP Apparatus main board, display pump and cuff damaged. Equipment installed on 26/10/2016 & aged up to 7+ years. Spare cost didn't received since spares are not available in market. Hence recommended for Condemnation
17	Name & Signature of CYRIX Authority	LIBIL LAL. 


*Not mandatory **#Based on the period of life and value as per the BER guidelines**

* **Attach Photograph**

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Main board, display, cuff, bladder damaged. Hence recommended for BER.






 19/01/24
 Signature of JC BM (Biomedical Engg) Consultant (NHM), Palakkad
 NHM (Arogya), Palakkad



Date 19/01/2024

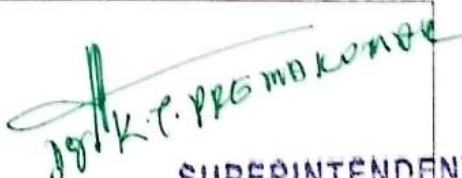
 SUPERINTENDENT
 Govt. W&C Hospital
 Palakkad
 Signature of
 Superintendent / Medical Officer (i/c)

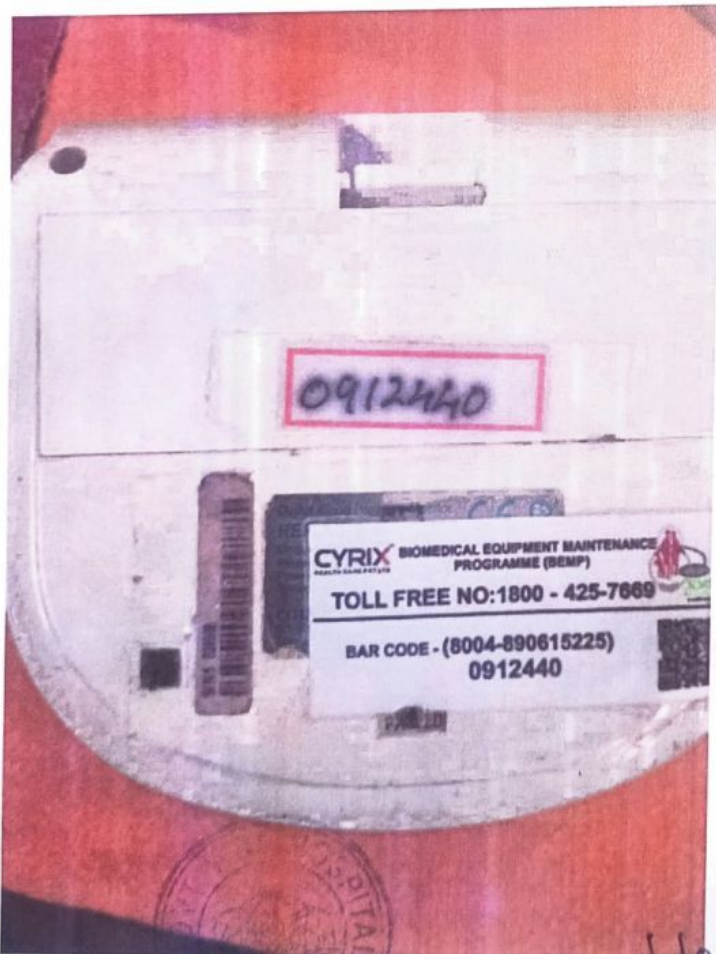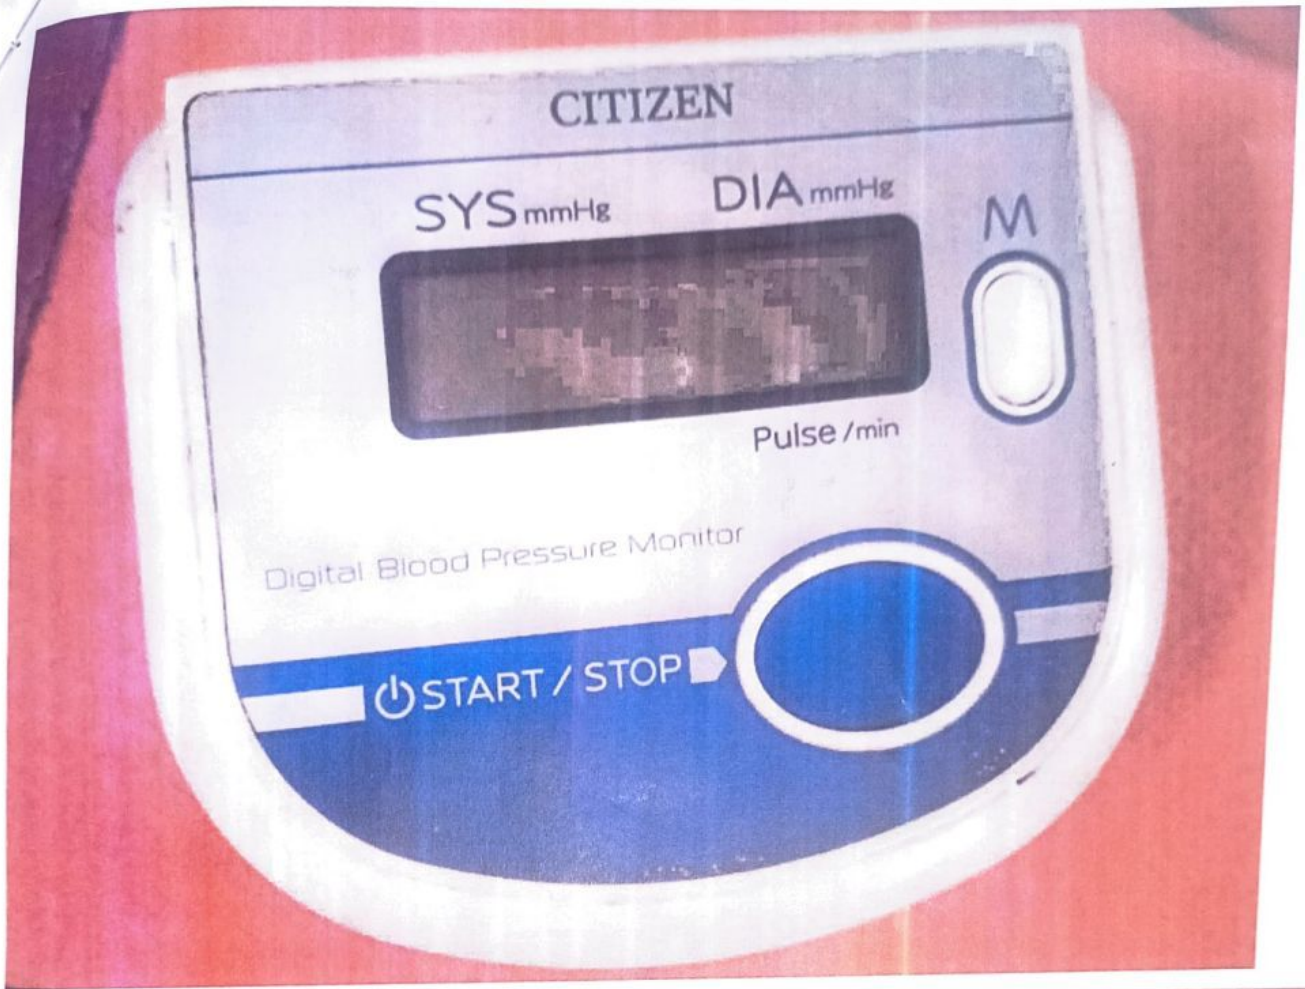

19/1/24

REENA-C.S
SND, ANW

SUPERINTENDENT
Govt. W&O Hospital
Palakkad

25/2/17

This is certified that the Book
contains 364 Pages serially numbered.

Reena
SNO

Inspected up to
31/8/16

[Signature]
Store Verification Officer
Dist. Medical Office (Health)
Palakkad

[Signature]

W&C HOSPITAL PALAKKAD

ANW

Instrument & furniture register

Code:

F volume: 1

FURNITURE & INSTRUMENTS
STOCK BOOK

Verified up to 31/12/19
July 19

[Signature]
Store Verification Officer
Dist. Medical Office (Health)
Palakkad

VERIFIED
UP TO

31/10/18

Checked
up to 31/3/2022

[Signature]
Store Verification Officer
Dist. Medical Office (Health)
Palakkad

P. Anil Kumar
Store Verification Officer (Incharge)
District Medical Office of Health
Civil Station-Palakkad

[Signature]

19/1/24

Reena.C.S

REENA.C.S
SNO, ANW



[Signature]
SUPERINTENDENT
Govt. W&C Hospital
Palakkad

1

INDEX

	III	Page no	
1. IRON COT.		3	INSTRUMENT TROLLY 85
2. STETHESCOPE		7	2 TWO TALK - (35)
3. LABOUR. COT		9	THERMOMETER 37
4. ✓ EXAMINATION TABLE		11	GILVOMETER (89)
5. ✓ FOOT STEP		13	WHEEL CHAIR (29)
6. STRUCTURE TROLLY		15	DIGITAL BP APPARATUS (60)
7. ✓ CEILING FAN		17	EMERGENCY LIGHT 49
8. ✓ IRON TABLE & DRAWER		25	STEEL TRAY ZLD 50
9. ✓ IRON STOOL		27	KIDNEY TRAY - 61
10. Wooden chair & Arm		29	CHEETAL FORSEPS-62
11. ✓ Wooden Bench		31	ARTERY FORSEPS-64
12. Lock & Key		33	SUTURE CUTTING SCISSORS CURVED (66)
13. ✓ Perforated chairs (Airport model)		41	SCISSORS ST' - 70
14. NEBULIZER & ACCESSORIES		51	STEEL BOWEL SMALL
15. ✓ Wooden table & Draw		53	8 MEDIUM - 72
16. ✓ Acquegard Valve		53	STAINLESS STEEL
17. Fetal Doppler		69	TRAY (3 BUCKETS) P.No-83 Clear
18. O ₂ FLOW METER & HUMIDIFIER		71	FETAL MONITOR
19. IV STAND		73	CTO MACHINE - 5
20. O ₂ Cylinder B (type)		65	STAINLESS STEEL B/W 23
21. NEEDLE DESTROYER		77	WALL FAN - 84
22. Industrial coil (Sterilizer coil)		85	FETAL DOPPLER (93)
23. BP Apparatus		81	Wooden stool - 98
24. ✓ STEEL RACK		45	Multisens (bed) - 95
25. ✓ PENESTIAL FAN		21	Shoe Rack 100
26. ✓ Steel Diarrhea		113	MULTIPARAMETER 103
27. Weighing Machine		55	CRASH CAR 105
28. Pet Jar (Plastic)		39	Ambu Bag (adult) - 107
29. Feet scope		57	Pulse oximeter - 109



SUPERINTENDENT
Govt. W & G Hospital
Palakkad

19/1/24

REENA - C.S
SNO, ANW

