



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 175247

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>District Hospital</u></p> <p>Address <u>Palakkad</u></p> <p style="padding-left: 150px;"><u>Kerala</u></p> <p>Ph : <u>94467889799</u></p>	<p>Call Registration Date : <u>12/01/2024</u></p> <p>Caller ID : <u>90241</u></p> <p>Date of Visit : <u>13/01/2024</u></p> <p>Asset No. : <u>0911233</u></p> <p>EQPT Name : <u>Pharmacy Refrigerator</u></p> <p>Manufacture <u>Electralux</u> Model : <u>ER 110D</u></p> <p>S. No. <u>Na</u> Dept. <u>Laboratory</u></p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not getting cool and

..... compressor damaged

Action Taken : Checked the equipment and found refrigerator

..... not getting cool and compressor damaged. Enquired spare with

..... vendor

Completed Date : 13/01/2024 Time : 12:30 pm

Spare Replaced Requested Spare Required

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrlix Engineer	Date	Start Time	End Time
<u>Muhammed lybal</u>	<u>13/01/24</u>	<u>11:50 am</u>	<u>12:30 pm</u>

Customer Remark Kindly requesting 800 RBER

Completed Pending


<p>Service Engineer Name : <u>Muhammed lybal</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>13/01/2024</u></p> <p>Contact Number : <u>7025548890</u></p>	<p>Customer Name : <u>PONTOUSHA J R</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>13/01/2024</u></p> <p>Contact Number : <u>9447889799</u></p> <p>Designation : <u>Deputy Director of Health Services & Superintendent.</u></p> <p>Hospital Seal : <u>District Hospital, Palakkad</u></p>
--	--

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	PALAKKAD
2	Name of Hospital	DH PALAKKAD
3	Name of Equipment with Make, Model and Serial Number	PHARMACY REFRIGERATOR MAKE: ELECTROLUX MODEL: ER 190D S/N: N/A
4	Equipment ID & Barcode	90341/ 0911233
5	Date of purchase / Year of manufacture /Installation Date	16-02-2006
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	12-01-2024 (TOLL FREE)
9	Action taken	Checked the unit, found refrigerator not getting cool, compressor damaged. Enquired spare with vendor.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendation
12	Cost of spares (specify parts and cost)	190 Liter fridge compressor: 3800 Cooling coil: 1750 Gas refilling charge: 3500 Inner condenser: 850 Total: 9900


13	Asset Value	9600
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	103.12%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report and quotation attached
16	Reasons for recommending the equipment as BER	After thorough examination, it was observed that the equipment's inner condenser tube is leaking, rendering it irreparable. Additionally, both the compressor and cooling coil are defective, necessitating gas filling. Considering the equipment's installation date of 16-02-2006 and its 17-year life span, it has exceeded its expected longevity. The cost of repairing the equipment surpasses its original asset value of rupees 9600, meeting the criteria for condemnation. Therefore, it is recommended to condemn the equipment based on its extensive wear, outdated technology and impractical repair cost.
17	Name & Signature of CYRIX Authority	Muhammed Iqbal 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Machine installed on 16-2-2006 and aged up to 17-years. The cost of the repairing cost exceeds the actual price of the machine hence recommended for BER.

Consultant (Biomedical) Engg
NHM (Aranya, Palakkad)

31-01-24
Signature of JC BM (NHM)


M. J. S. R.
SENIOR ORGANO-LABORATORY TECHNICIAN




V. Jayasree

Signature of Director of Health Services
Superintendent, Deputy Medical Superintendent,
District Hospital, Palakkad.

Date

Seal

BHARATH **REFRIGERATION**

DOOR NO. 18, MINI INDUSTRIES,
KALMANDAPAM, PALAKKAD - 678 001

Repairing & Servicing Of :-
REFRIGERATORS
AIR CONDITIONERS
DEEP FREEZERS
WASHING MACHINES
CHILLERS, COOLER

Ref:


Date : 30/1/24

Quotation for fridge Repairing



Mr cyrus Health Care
Cochin.

1	190 Lt Fridge Compressor replacement charge	3800.00
2	Cooling Coil replacement	1750.00
3	Gas refilling charge with driver, working charge	3500.00
4	Lower Condenser replacement charge	850.00
5	to and fro charge	400.00
		<u>10300.00</u>

(Prices Tentative thru market)

For Bharath Refrigeration


Proprietor

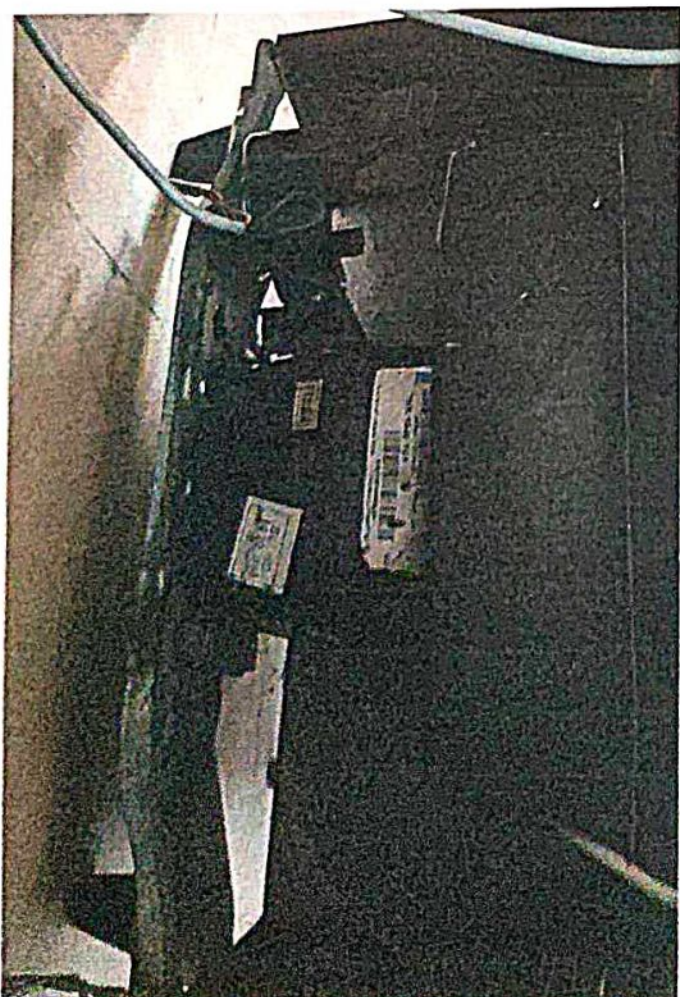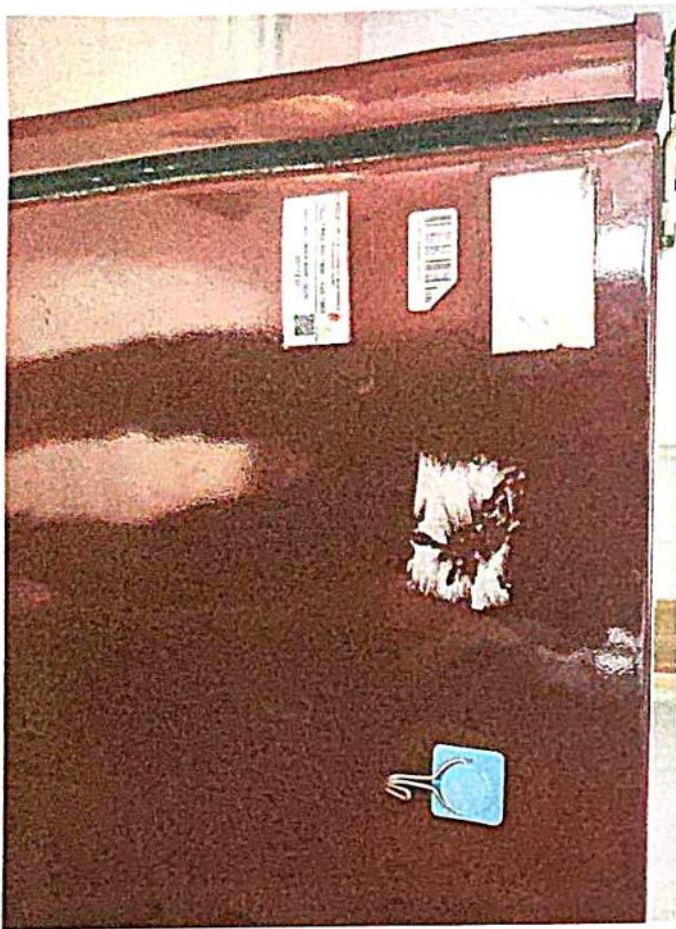

Vijayar
Deputy Director of Health Services
& Superintendent,
District Hospital, Palakkad.
Dist. Health Officer
GOVT. OF KERALA

RERRIGERTOR.



31.1.06	Store Supdt Dist Hospital Palakkad. Stock books etc 129 Old refrigerators in warranty period Expired, not working. Capacity 300 lit. Godrej Ultra. Report of. S.No. RCDMP of 2006	1		1 F	
16.2.06	S.S. Dh. Pkd	1.5		1.5	
	Electrolux Refrigeration 180L. Rs. 8400/- 5 years warranty	1 F		2 F	
	V. Guard Stabilizer 500VA Rs 1000/-	1.5		2.5	
	Fridge Stand Rs 200/-	1*			
	Total 9600/-		2 F + 1.5	NIL	2 F + 1.5
17.2.06	Used in late				
29.5.06	Electrolux Refrigerator	4 F		6 F	
	Store Supdt Dist Hospital Pkd				
	Capacity Rs 9672/- per one. Warranty				
	V. Guard Stabilizer Rs 924/44 per one.	4.5		6.5	
30.5.06	Used in late		4 F + 4.5	NIL	6 F + 6.5
	1 - Bio				
	1 - Histo				
	1 - CP				
	1 - Endo				
	1 - comp (Cammela)				
	1 - Store				

Vijayan
Deputy Director of Health
& Superintendent,
District Hospital, Palakkad