


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL
EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KASARGOD
2	Name of Hospital	CHC KUMBLA
3	Name of Equipment with Make, Model and Serial Number	SEMI AUTO BIOCHEMISTRY ANALYZER MAKE: ROBONIK MODEL: PRIESTEST TOUCH S/N: AT0120313RBK
4	Equipment ID & Barcode	92712 & 1430390
5	Date of purchase / Year of manufacture / Installation Date	14-08-2013
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email / Toll free)	25-01-2024 (Toll free)
9	Action taken	Checked and found the main PCB and display defective. Need to replace main PCB and display for further checking of the complaint. Quotation enquired.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendation.
12	Cost of spares (specify parts and cost)	N/A


13	Asset Value	64760
14	#PercentagevalueofthecostofspareswithrespecttoCostofPurchase/Asset Value	N/A
15	Abstract of Service Report provided bythe OEM/ Authorized Service Provider/CYRIX(AttachedorNot)	CYRIX SERVICE REPORT AND OEM LETTER ATTACHED.
16	Reasons for recommending theequipment as BER	Checked and found main PCB and Display are defective. Equipment installed on 14-08-2013 and aged up to 10 years 5 month, life span of the equipment used. As per OEM report this model is obsolete, not repairable and spare not available. So we recommending the unit for condemnation.
17	Name&SignatureofCYRIXAuthority	AJITH BABU K 

*Notmandatory #BasedontheperiodoflifeandvalueaspertheBERguidelines


*AttachPhotograph

RemarksandRecommendationsofJuniorConsultant(Biomedical)NHM:

Checked the machine and found Problem with main PCB & display. Equipment installed on 14/08/2013. OEM letter attached. AS Per OEM letter, this model declared as End of Life.


 16/02/24
SignatureofJCBM(NHM)

Biomedical Engineering
Arogyakeralam (NHM)
Kasaragod at Kanhangad

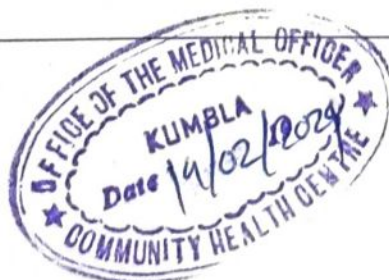

Date

Seal


for Ms. Dr. Deepthi
Dr. Deepthi

Signature of
Superintendent/Medical Officer(i/c)
MEDICAL OFFICER
COMMUNITY HEALTH CENTRE KUMBLA
KASARAGOD DIST.-671321



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 185857

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>SHC Kumbala</u></p> <p>Address <u>Kasaragod</u> <u>Kerala</u></p> <p>Ph : <u>9496104896</u></p>	<p>Call Registration Date : <u>25-1-24</u></p> <p>Caller ID : <u>98712</u></p> <p>Date of Visit : <u>27-1-24</u></p> <p>Asset No. : <u>1430390</u></p> <p>EQPT Name : <u>Biochemistry Analyzer</u></p> <p>Manufacture <u>Robarik</u> Model : <u>protected down</u></p> <p>S. No. <u>A.T.O.120313R4</u> Dept. <u>LAB</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Blue display

Action Taken : checked the machine and found problem with the primary board and display, need to replace the primary board and display for checking further working condition of the machine

Completed Date : 6-2-24 Time : 2:00 PM Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number



Cyrix Engineer	Date	Start Time	End Time
<u>Ajith</u>	<u>6-2-24</u>	<u>1:00 PM</u>	<u>2:00 PM</u>

Customer Remark: Completed Pending

<p>Service Engineer Name : <u>Ajith Baburik</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>6-2-24</u></p> <p>Contact Number : <u>8848079288</u></p>	<p>Customer Name : <u>Dr. Deepthi</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>6/2/24</u></p> <p>Contact Number : <u>9496104896</u></p> <p>Designation : <u>Lab technician grade I</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
---	---

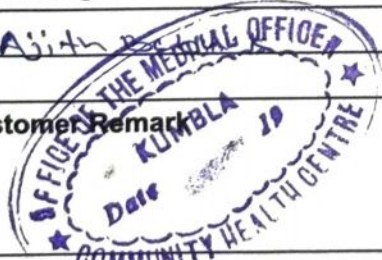

MEDICAL OFFICER
KASARAGOD DIST. OFFICE
Dr. Deepthi
Dr. Remya Raveend

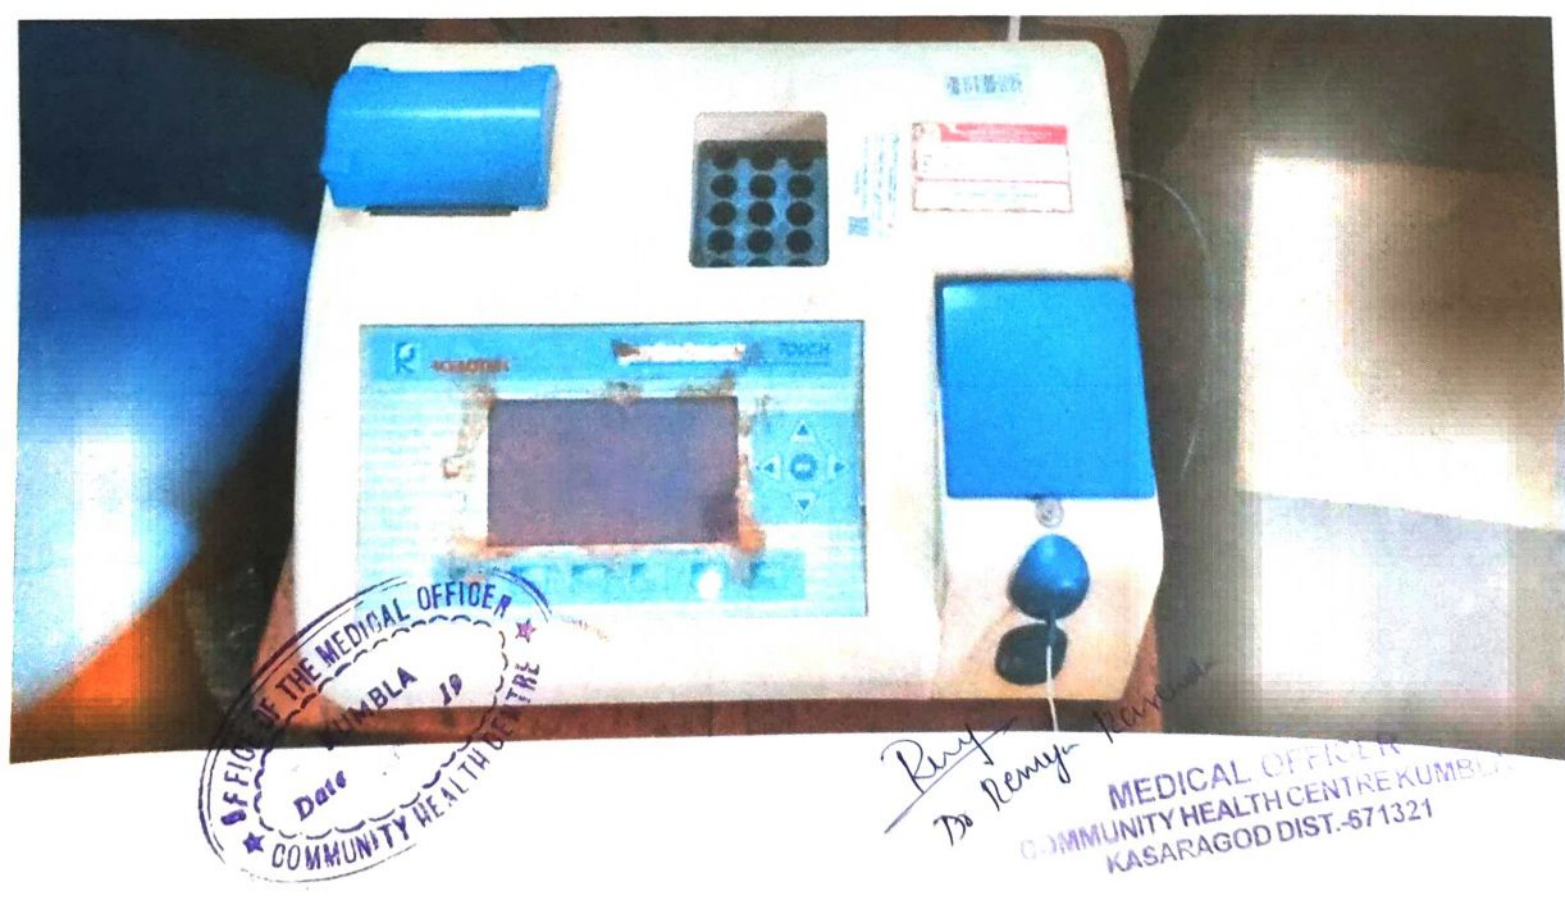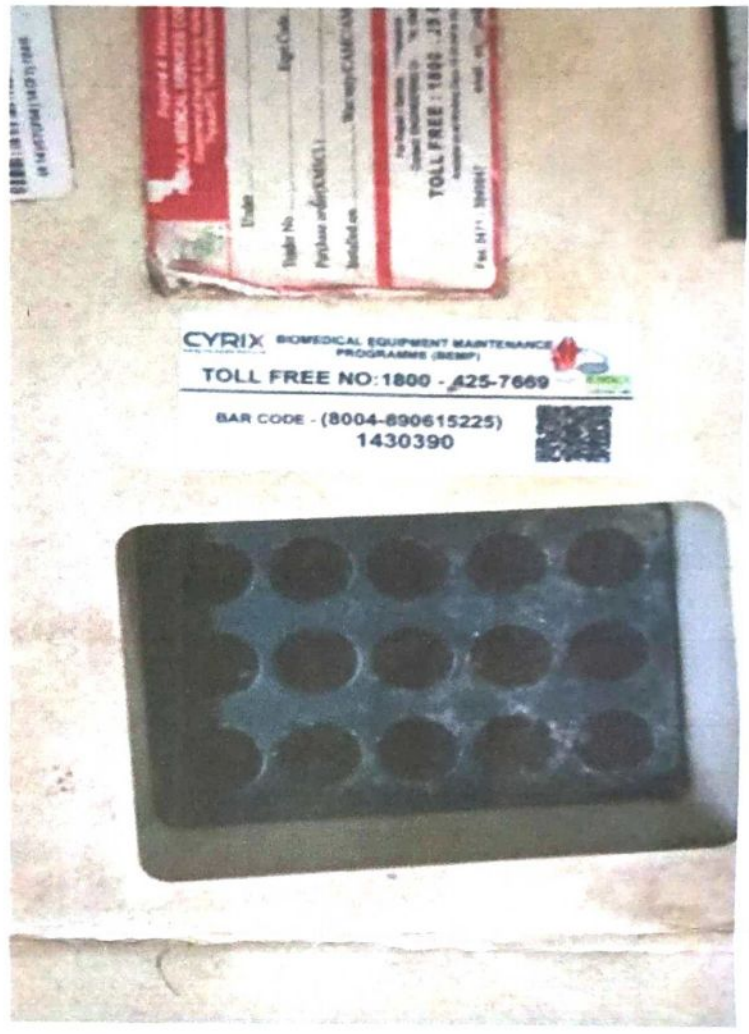

Community Health Centre, Kumbla 123

Month	Opening Balance	Receipt	Total	Issued	Balance
		<u>BIOCHEMISTRY ANALYSER</u>			
06/08/13		BIOchemistry Analyser - Robonic. Model - Parietest Touch Serial No: AT 0120313 RBK		1 Installed on 14/8/2013	
27/8/13				1	
20/10/2019		Merit Diagnostic Private Lenited By asst Semi Automatic Biochemistry Analyser. Serial No - CMB 021566 Rs 56,640.		1	2
		CLINICANT MICRO C Dry bed incubator 37°C. Bathy Block UPS.		1x6 1x6	

Remy
Dr Remy, Raveendran

MEDICAL OFFICER
COMMUNITY HEALTH CENTRE KUMBLA
KASARAGOD DIST.-671321



Date: 30th January 2023

Dear Valued Customer,

Thank you for choosing **Robonik (India) Pvt Ltd**. We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having **Serial No. AT0120313RBK**.

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having **Serial No. AT0120313RBK** as **End of Life (EOL) Notified**. (Duration from installation is 10 Years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK INDIA PVT LTD**



AUTHORIZED SIGNATORY