


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	PALAKKAD
2	Name of Hospital	CHC VADAKKENCHERY
3	Name of Equipment with Make, Model and Serial Number	SEMI AUTO BIOCHEMISTRY ANALYZER MAKE: ROBONIS MODEL: PRIESTEST TOUCH SN : AT028085RBLQ
4	Equipment ID & Barcode	87009, 0930368
5	Date of purchase / Year of manufacture / Installation Date	14 / 03 / 2015
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC / NO CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	22 / 12 / 2023, TOLL FREE
9	Action taken	Checked and found that main PCB, Flow cell defective. Need to replace main PCB and Flow cell for further checking of complaint required for spare
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged.
11	Recommendations for repair (required service details)	No recommendation
12	Cost of spares (specify parts and cost)	


13	Asset Value	67998
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX service report OEM letter attached
16	Reasons for recommending the equipment as BER	checked and found that main PCB flow cell defective. Equipment installed on 14/03/15 and aged upto 6 year 9 month life span of the equipment used. As per OEM report this model is obsolete model not repairable and spare not available. Both RBER criteria met. So we recommended for condemnation.
17	Name & Signature of CYRIX Authority	D NINIK D

*Not mandatory #Based on the period of life and value as per the BER guidelines

* **Attach Photograph**


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Main board and flow cell defective.
Hence recommended for BER.



[Signature]
27/01/24
Signature of JC BM (NHM)

Date _____ Seal _____



[Signature]
For Dr. Sreeja
Signature of
Superintendent / Medical Officer (i/c)
Superintendent
Community Health Centre
Vadakkencherry, Palakkad



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 175453

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>P.H.C. YADAKKENCHERY</u></p> <p>Address <u>YADAKKENCHERY</u> <u>PALAKKAD</u></p> <p>Ph : <u>9947078586</u></p>	<p>Call Registration Date : <u>22/12/23</u></p> <p>Caller ID : <u>83009</u></p> <p>Date of Visit : <u>24/12/23</u></p> <p>Asset No. : <u>0430368</u></p> <p>EQPT Name : <u>SEMI AUTO BIOCHEMISTRY ANALYZER</u></p> <p>Manufacture <u>ROBONIS</u> Model <u>PRIESTEST TOUCH</u></p> <p>S. No. <u>AT0280315RBK</u> Dept. <u>LABORATORY</u></p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Machine not working.

Action Taken : Checked the machine. Found that main PCB and flow cell defective. Need to replace main PCB and flow cell for further checking of complaint enquired for spare.

Completed Date : 27/01/24 Time : 11:30 AM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. <u>Nil</u>			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>DIVINIS</u>	<u>27/01/24</u>	<u>10:00 AM</u>	<u>11:30 AM</u>

Customer Remark Completed Pending

<p>Service Engineer Name : <u>DIVINIS</u></p> <p>Signature : </p> <p>Date : <u>27/01/24</u></p> <p>Contact Number : <u>9847299500</u></p>	<p>Customer Name : <u>LINI V.K</u></p> <p>Signature : </p> <p>Date : <u>27/01/24</u></p> <p>Contact Number : <u>9846789669</u></p> <p>Designation : <u>Lab Technician</u></p> <p>Hospital Seal : </p>
---	---



Abani
Superintendent
Community Health Centre
Vadakkanchery

Date : 12th January 2024

Dear Valued Customer,



Thank you for choosing **Robonik (India) Pvt Ltd**. We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having **Serial No. AT0440315RBK / AT0280315RBK**.

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model: Prietest Touch) having **Serial No. AT0440315RBK / AT0280315RBK** as **End of Life (EOL) Notified**. (Duration from installation is 08 Years).




Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK INDIA PVT LTD**



AUTHORIZED SIGNATORY

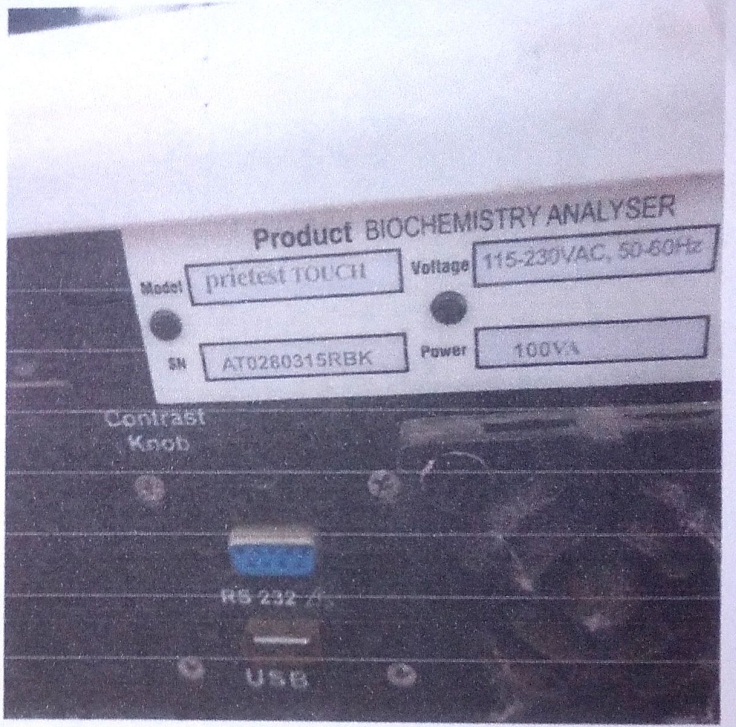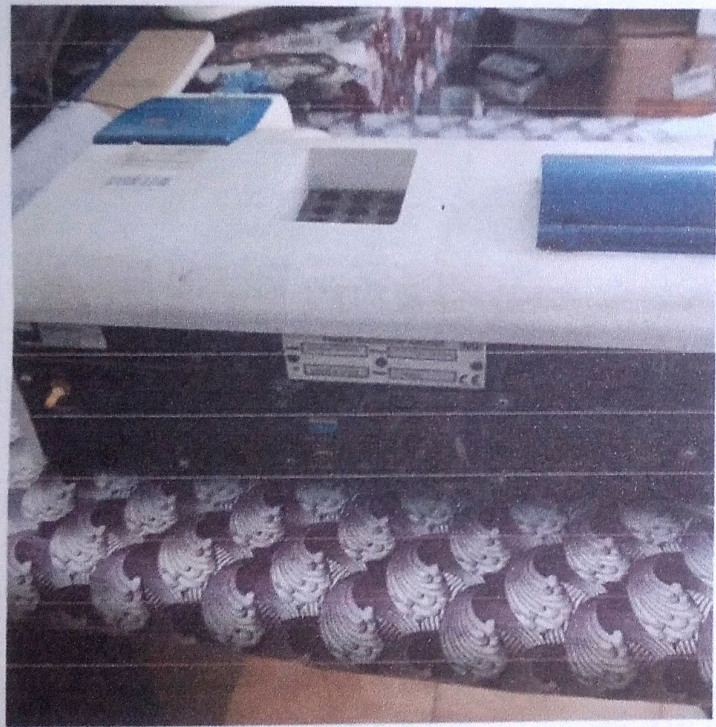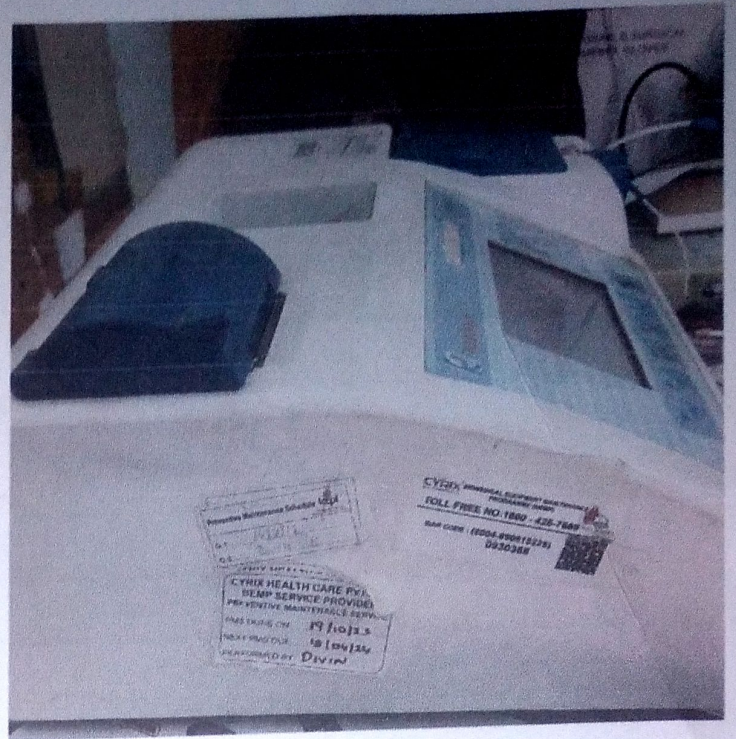

Charan

For: Dr. Sreeja

**Superintendent
Community Health Centre
Vadakkencherry, Palakkad**

16

BIOCHEMISTRY ANALYSIS

Date

Referred From

Ref: PUSONIK & UPS
(React) / Balum

14/3/15

KMSCL - M

SINO. AT. 0280315RBK

1 no.

Rs 67998/-

JNVac. no - 251



Abiraj

For: *Dr. Sreedan*
Superintendent
Community Health Centre
Vadakkancherry, Palakkad