


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KANNUR
2	Name of Hospital	FHC CHITTARIPARAMBA
3	Name of Equipment with Make, Model and Serial Number	SEMI AUTO BIOCHEMISTRY ANALYZER Make: ROBONIK Model: PRIETEST TOUCH SN: AT1681013RBK
4	Equipment ID/ Barcode	1345236 #101036
5	Date of purchase/ Year of manufacture/Installation Date	27-11-2013
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free 13-03-2024
9	Action taken	Checked the machine and found that Machine is not switching ON, found problem with primary board, enquired OEM for quotation
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	N/A

13	Asset Value	64760/-
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report & OEM End of life letter attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that Machine is not switching ON, found problem with primary board, enquired OEM for quotation. Equipment installed on 27-11-2013 aged up to 10 years 3 Months, oem informed that this machine is obsolete model, end of life letter issued. As per tender clause 5.3.14.2 we recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AVINASH T 


*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


checked & identified that machine not working and aged up to 10 years above. As per OEM the machine is obsolete model and end of life letter received. So recommended for BER as per BER protocol.


Signature of JC BM (NHM)
22/03/24

Recommending for Condemnation

Date: 25/03/24



Signature of 
Superintendent/Medical Officer (BER)

25/3/24

MEDICAL OFFICER
PRIMARY HEALTH CENTRE
CHITTAMPARAMBA
P. O. KANNOTH-670 650



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 189383

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility pbc chittaxi paramba</p> <p>Address Kanner</p> <p style="padding-left: 100px;">Kerala</p> <p>Ph : 7510237592</p>	<p>Call Registration Date : 13-3-24</p> <p>Caller ID : 101036</p> <p>Date of Visit : 14-3-24</p> <p>Asset No. : 1345236</p> <p>EQPT Name : Semi auto biochemistry Analyser</p> <p>Manufacture Robonik Model : prietestouch</p> <p>S. No. AT1681013RBK Dept. laboratory</p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Equipment is not switching on.

Action Taken : checked the equipment and found that equipment is not switching on. Found problems with primary board Enquired OEM for quotation.

Completed **Date :** 14-3-24 **Time :** 12:45pm **Spare Required**

Spare Replaced **Requested**

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Shyamkishan ppk	14-3-24	11:40 am	12:45 pm

Customer Remark Completed Pending

<p>Service Engineer Name : Shyamkishan ppk</p> <p>Signature : </p> <p>Date : 14-3-24</p> <p>Contact Number : 8281188514</p>	<p>Customer Name : Shafana V.K</p> <p>Signature : </p> <p>Date : 14/3/24</p> <p>Contact Number : 7510237592</p> <p>Hospital Seal : LT M-I</p>
---	--

Date : 15th March 2024

Dear Valued Customer,



Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1681013RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1681013RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**




Authorised Signatory




STOCK BOOK (MEDICINES)

Name of drug Automatic Biochemistry Analyser

Date	Receipt	Issue	Balance	Date	Receipt	Issue	Balance	Remarks
	kg./gm./ml.	kg./gm./ml.	kg./gm./ml.		kg./gm./ml.	kg./gm./ml.	kg./gm./ml.	
27.11.13							NIL	
No. 2473	Received from KMBCI.							
25.10.13	The instrument is received from KMBCI				1 NO		1 NO	
	Accessories:-					1 NO	NIL	
	1. Sine wave UPS				1 NO			
	2. Halogen Lamps				1 NO			
	3. Thermal Print Paper				02 NO			
	4. Dust Covers				1 NO			Issued to ✓
	5. Variable volume Pipette 10-100ml				1 NO			Lab ✓
	6. One fixed volume Pipette - 500ml				1 NO			
	Reagents:-							
	1. Urea mod				500ml x 1 bot			
	2. Creatinine				500ml x 1 bot			
	3. Billirubin TAD				500ml x 1 bot			Issued to ✓
	4. Cylucose				500ml x 1 bot			Lab ✓
	5. Cholesterol				500ml x 1 bot			
	6. Q.C. Abnormal				05ml x 1 bot			
	7. Q.C. Normal				05ml x 1 bot			
	S. No. 101 AT 118-1013 RBK				Mfg: Reborik Pvt Ltd. Chennai			
	Grand total Rs: 84521/-				Warranty 26.11.2016 (3 years)			
27.11.13	Issued to Lab technician						NIL	
	Stock entry page no. 104/vol III							

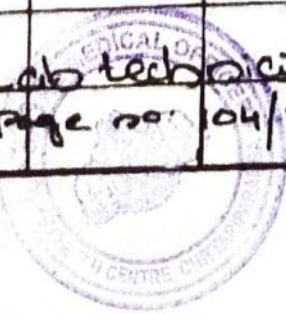

MEDICAL HEALTH CENTRE
 CHITTARIPARAMBA
 KANNOTH-670 650

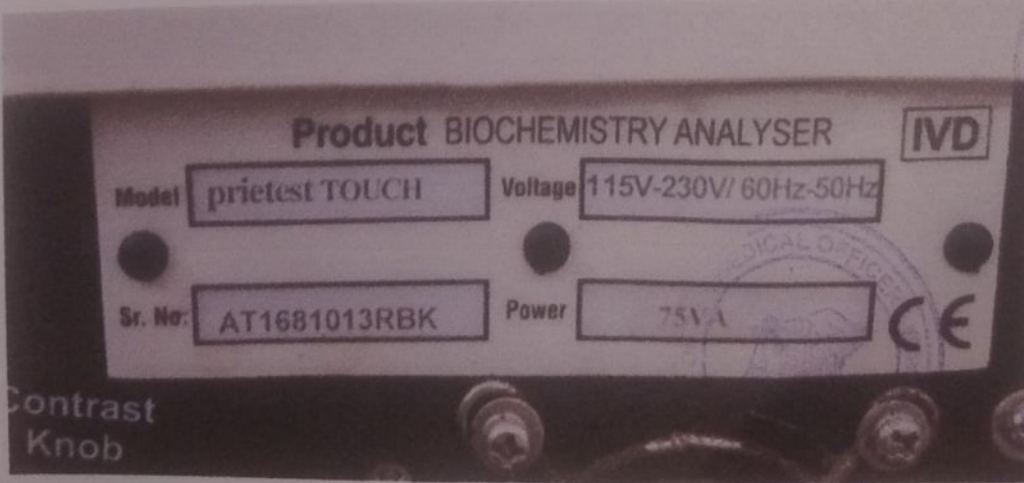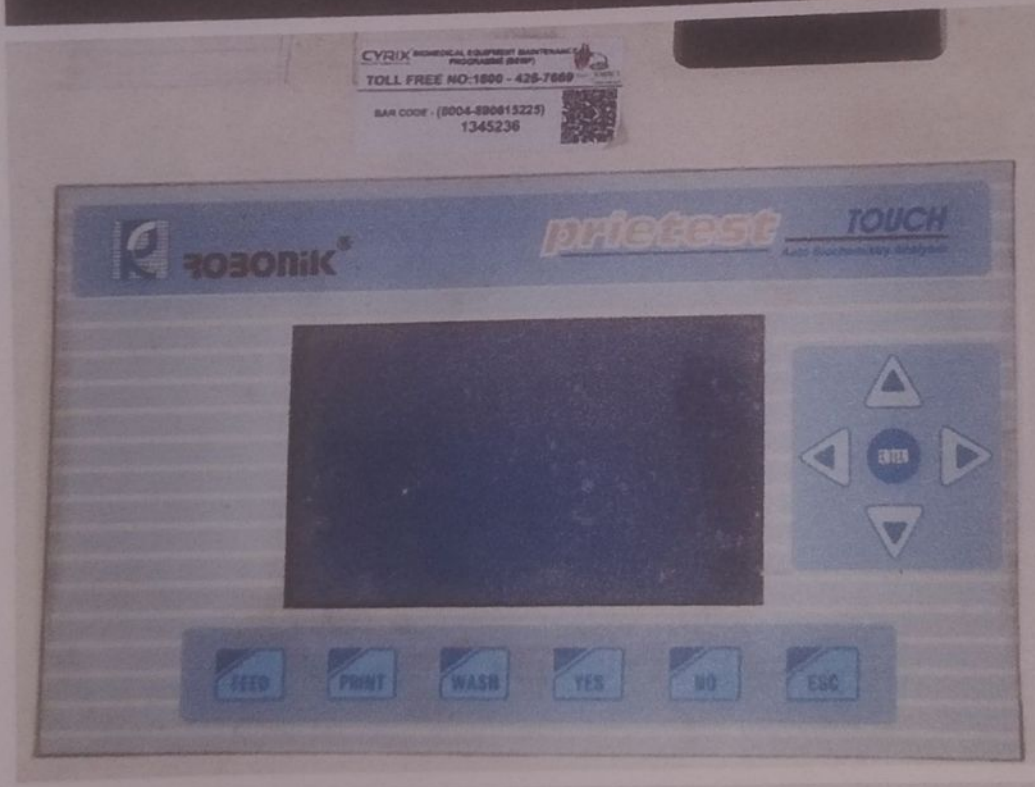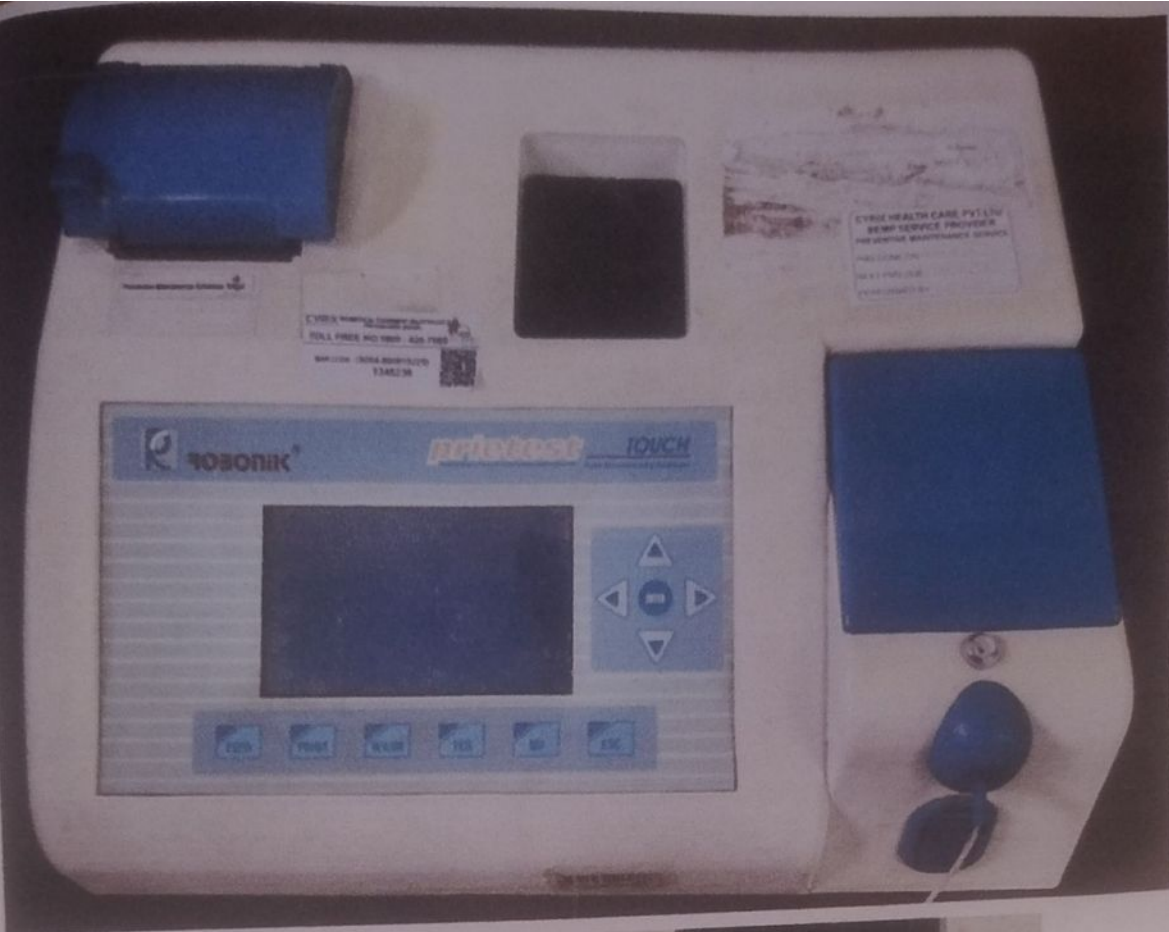

MEDICAL OFFICER
 GOVT HEALTH CENTRE
 TARIPARAMBA
 P. O. KANNOTH-676 859
 25/3/24