



**BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAMME  
UNDER  
NATIONAL HEALTH MISSION**



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

**CYRIX**  
HEALTHCARE PVT LTD

**No. : 193966**

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <i>THQH, Kayamkulam</i>	Call Registration Date : <i>21/03/2024</i>
Address <i>Aleppuzha</i>	Caller ID : <i>102562</i>
<i>Kerala</i>	Date of Visit : <i>22/03/2024</i>
Ph : <i>8606817608</i>	Asset No. : <i>0421040</i>
	EQPT Name : <i>ECG Machine</i>
	Manufacture <i>BPL</i> Model : <i>Cardiac 6108T</i>
	S. No. <i>AVMP3G-22058</i> Dept. <i>ECG Room</i>

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** *Not getting ON*

**Action Taken :** *Checked the machine and Found that the ECG Main PCB, Battery and printer Head Assembly are defective. Enquired the OEM for spares. Need to replace these spares for further checking and working condition of the equipment.*

Completed  Date : *22/3/24* Time : *2:00 pm* Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<i>Mardula G</i>	<i>22/03/24</i>	<i>12:30 pm</i>	<i>2:00 pm</i>

Customer Remark  Completed  Pending

Service Engineer Name : <i>Mardula G</i>	Customer Name : <i>Chinchi.v</i>
Signature : <i>Mardula G</i>	Signature : <i>Chinchi.v</i>
Date : <i>22/03/2024</i>	Date : <i>22/03/24</i>
Contact Number : <i>9081199471</i>	Contact Number : <i>8606817608</i>
	Designation : <i>ECG Technician</i>
	Hospital Seal :



*7*  
Govt. Taluk Hospital  
Kayamkulam





**BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAMME  
UNDER  
NATIONAL HEALTH MISSION**



SERVICE PROVIDER  
Tender No. WO-37/2021-2022/698

**CYRIX**  
HEALTHCARE PVT LTD

No. : 193916

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility	THQH, Kayamkulam	Call Registration Date :	21/03/2024
Address	Alappuzha Kerala	Caller ID :	102562
Ph :	8606817608	Date of Visit :	22/03/2024
		Asset No. :	0421040
		EQPT Name :	ECG Machine
		Manufacture	BPL Model : cardiast 108T
		S. No.	AVMP3G20058 Dept. ECG Room

**Service Classification :** Breakdown Call  PMS  Calibration  Cust. Training

**Problem Identified :** Not getting ON

**Action Taken :** checked the machine and found that the ECG Main PCB, Battery and printer Head Assembly are defective. Enquired the OEM for spares.

Completed  Date : 05/04/24 Time : 1:30 PM Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Mridula G	05/4/24	12:45 PM	1:30 PM

**Customer Remark** Completed  Pending   
Requesting for confirmation Chircheru V  
Chircheru 5/04/24

Service Engineer Name : Mridula G	Customer Name :
Signature : <i>[Signature]</i>	Signature :
Date : 05/04/2024	Date :
Contact Number : 9061199471	Contact Number :
	Designation : Superintendent
	Hospital Seal : Govt Taluk Hospital Kayamkulam




**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

Sl. No	Particulars	Details
1	Name of District	ALAPPUZHA
2	Name of Hospital	THQHKAYAMKULAM
3	Name of Equipment with Make, Model and Serial Number	ECGMACHINE MAKE :- BPL MODEL:-CARDIART6108T SN :- AVMP3G22058
4	Equipment ID& Barcode	102562&0421040
5	Date of purchase/Year of manufacture /Installation Date	31/08/2013
6	Warranty details(Yes/No)	NOWARRANTY
7	*AMC/CAMC Period agreed at the time Of purchase	NOAMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	21/03/2024
9	Action taken	Checked the machine and found that the ECG Main PCB, Battery & Printer Head Assembly are defective. Enquired the OEM for spares.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not Recommending for repair
12	Cost of spares(specify parts and cost)	Main PCB Assay 6108 T :-14000/- NIMH Battery 9.6V , 1.4Ah :- 2048/- <u>PrintHeadAssembly6108T:-2206.6/-</u> Total :-18254.6/-




13	Asset Value	RS:- 23391.38/-
14	#Percentage value of the cost of spares with respect to Cost of Purchase/Asset Value	78%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service Report & OEM Quotation Attached.
16	Reasons for recommending the equipment as BER	Checked the machine and found that the ECG Main board, Battery & Printer Head Assembly are defective. Enquired the OEM for Quotation. This equipment installed on 31/08/2013, aged upto 10 years and 7 months. Percentage of service cost is high (78%) and economically not viable. Both criteria met as per the tender clause 5.3.14.1 we are Recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	 MRIDULAG

\*Not mandatory #Based on the period of life and value as per the BER guidelines

\*Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical)NHM:

*Recommended for BER*


  
**JYOTHISH THOMAS**  
 Consultant (Biomedical Engineering)  
 NHM ALAPPUZA  
 Signatory of JCBM(NHM)

*Signature for Condemnation*

Date



Seal

  
 Signature of Superintendent/Medical Officer (i/c)

**Superintendent**  
 Govt. Taluk Hospital  
 Kayamkulam

ECG MACHINE

B/F page 13 3183  
 24.12.05 IN. No. 293/05-06 Dms Alappally machines 05080796 issued  
 Rs. 12500/each 1 1 Nil

22.2.06 issued to ECG Technician 1 Nil

- Power cord 3pin - 1
- Patient Cable (10 lead lead type) - 2
- Clamp electrodes - 1 set
- Chest Electrodes with Bullans - 6 Nos
- ECG Jelly bottle - 2 Nos
- Earthing Cable - 1 no
- Paper Roll 55mm - 1 no
- User's manual - 1
- Warranty card - 1
- Baluru Nil

5/6/13 W.No: CAM/FG/98/13-14 dtd 31.05.2013 from BPL Limited  
 No. 35-261, Milma dairy, Meethanar Road, Koonamthai, Edappally, Cochin

BPL ECG MODEL 6108T ① 23,450.00  
 one pmt tax - VAT @ 5% 1,172.50  
24,622.50

Issued to ECG Technician 1 Nil  
 Baluru Nil

Received  
 Shreejith

2 21.8.2013 W.No: EKM/FG/203/13-14 dtd 23/Aug/2013 from BPL Ltd No: 35-261  
 Milma dairy - Meethanar Road, Koonamthai, Edappally, Cochin

1. BPL ECG MODEL 6108T ① 22,299.00  
 one pmt tax - VAT @ 5% 1,113.88



Issued to ECG Technician 1 23,391.38  
 Baluru Nil


Received  
 Shreejith  
 P. G. T. K.

C/O to 134

Superintendent  
 Govt. Taluk Hospital  
 Kayamkulam



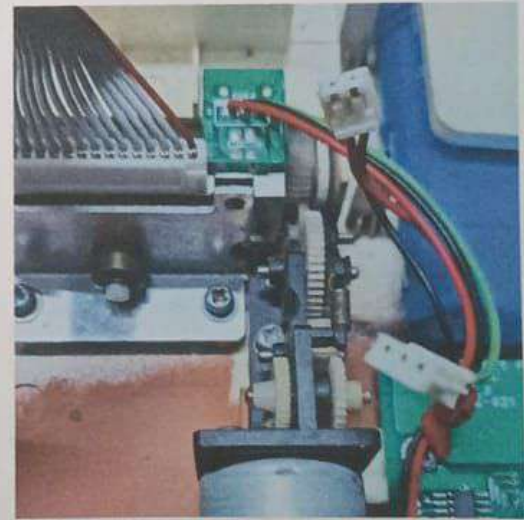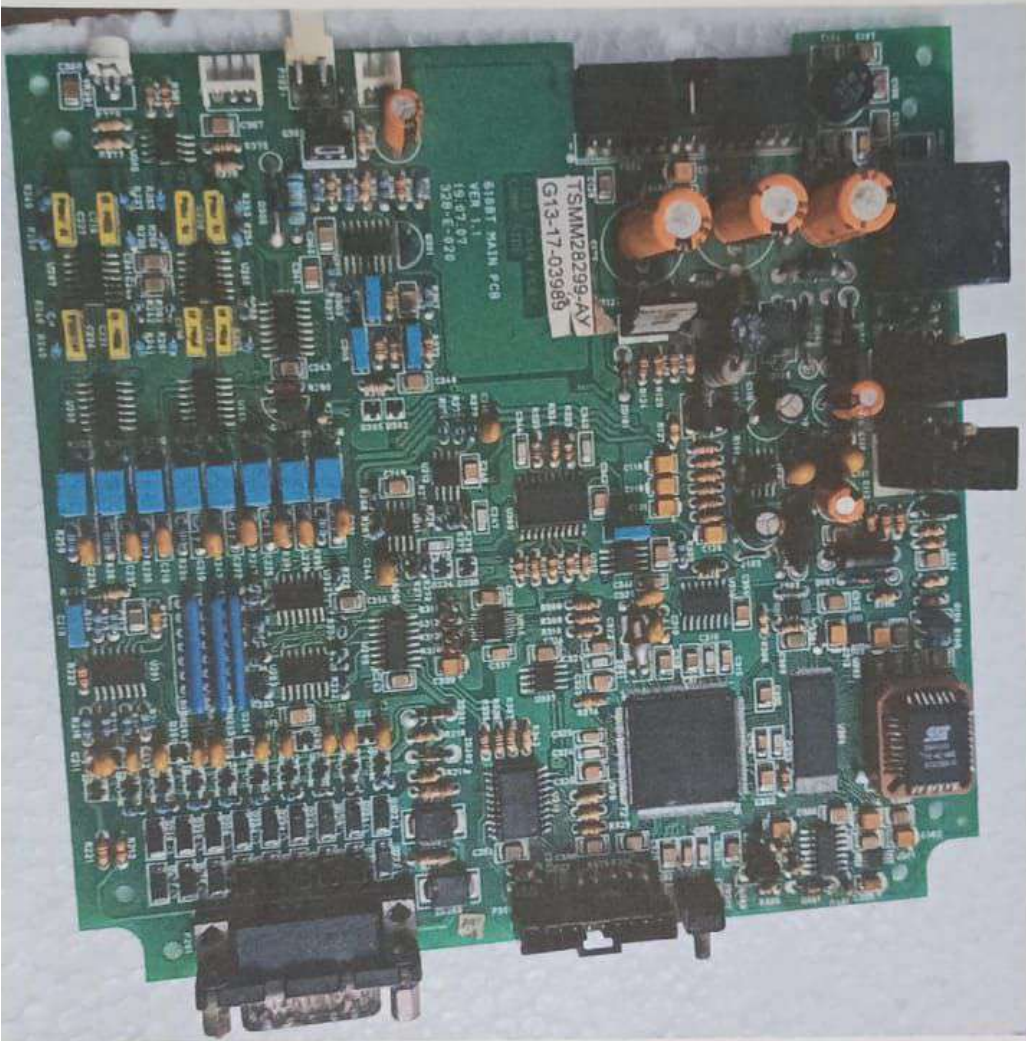

  
 Superintendent  
 Govt. Taluk Hospital  
 Kayamkulam



QTN/BISO/050424-002

05/04/2024

**QUOTATION**

To,  
CYRIX HEALTH CARE PVT LTD  
ERNAKULAM

Dear Sir,

Please find below our lowest quotation for the following items:-

SL NO.	ITEM DESCRIPTION	COST PER UNIT	UNIT PRICE
1	ECG 6108T MAIN PCB ASSY NEW (WITH LPC IC)	12500	12500+12%TAX
2	BM/OM NIMH BATTERY 9.6V 1.4 AH	1600	1600+28%TAX
3	PRINT HEAD ASSY 6108T	1870	1870+18%TAX

Terms and conditions:

1. Payment 100% in advance along with Purchase order
2. Delivery within 15 days

Thanking you and assuring you our best attention always.

For Biomedix Solutions




Authorized Signatory

Mobile: 9846969564 | Email: [biomedixservice@gmail.com](mailto:biomedixservice@gmail.com)

Branches: Kozhikode, Kannur, Kottayam-Kollam.

For enquiries contact: [biomedixsales@gmail.com](mailto:biomedixsales@gmail.com), [biomedixservice@gmail.com](mailto:biomedixservice@gmail.com)



BIOMEDIX SOLUTIONS

No: 7/437- B, Mannarakayam P.O,  
Kathilankalpadi, Kanjirapally, Kottayam - 686506,  
Mob:9846969564,