


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	Kottayam
2	Name of Hospital	THQH Vaikom
3	Name of Equipment with Make, Model and Serial Number	Name of Equipment : Nebulizer Make : Aerosol SN : 00152
4	Equipment ID & Barcode	0521275 , 96735
5	Date of purchase / Year of manufacture /Installation Date	16 / 9 / 2014
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	18 / 2 / 2024
9	Action taken	checked the machine motor Fully damaged.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Major part (motor) of the machine fully damaged.
12	Cost of spares (specify parts and cost)	Equal to Asset value

13	Asset Value	2950
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	Equal to Asset value
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Service report and damage part photo attached.
16	Reasons for recommending the equipment as BER	Major part of the machine (motor) fully damaged. This reasons for recommending the equipment as RBER.
17	Name & Signature of CYRIX Authority	Josekutty George 

*Not mandatory **#Based on the period of life and value as per the BER guidelines**

* **Attach Photograph**

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Asset value - 2950
 Cost of spare = equal to Asset value
 life period (installed 16/9/14) of years
 The machine fully damaged - as per the
 RBER guidelines recommended as RBER


 Signature of JC BM (NHM)

Date



Seal


 Signature of Superintendent / Medical Officer (i/c)

28/1/24
 Superintendent
 Taluk Head Quarters Hospital
 Vaikom. Pin - 686 111

**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 180521

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <u>THQH Vaikom</u>	Call Registration Date : <u>18/2/2024</u>
Address <u>Kottayam</u>	Caller ID : <u>96735</u>
Ph : <u>9947002147</u>	Date of Visit : <u>21/2/2024</u>
	Asset No. : <u>0521275</u>
	EQPT Name : <u>Nebulizer</u>
	Manufacture <u>Aerosol</u> Model : <u>NA</u>
	S. No. <u>0052</u> Dept. <u>ward-4</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : checked the machine motor damaged motor not repairable.

Completed Date : 21/2/2024 Time : 12 pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. RBER			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Josekutty George</u>	<u>21/2/2024</u>	<u>11:30am</u>	<u>12 pm</u>

Customer Remark Completed Pending



Service Engineer Name : Josekutty George
Signature : [Signature]
Date : 21/2/2024
Contact Number : 8898230907



Customer Name : Basheera Begum Poyan
Signature : [Signature]
Date : 21/2/24
Contact Number : 9947002147
Designation : Nurse In Charge OFFICER
Hospital Seal :



CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225) 0521275

AEROSOL COMPRESSOR
Filter
Outlet
Switch

1204
CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225) 0521275

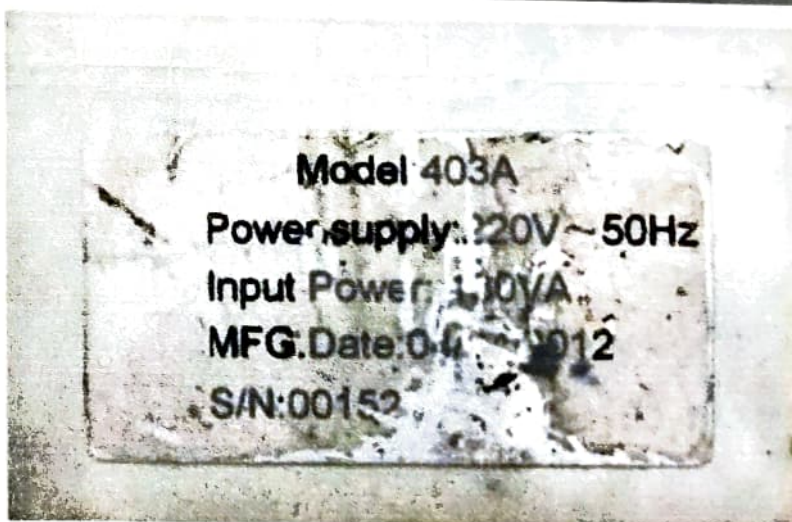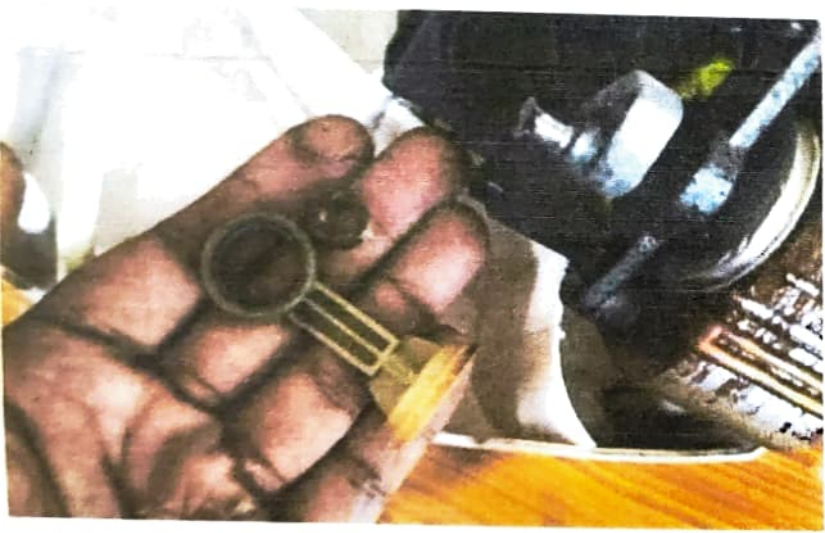

Model 403A
Power supply: 220V ~ 50Hz
Input Power: 1.10VA
MFG. Date: 04 / 2012
S/N: 00152



CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225) 0521275

Nebrulizes

	Recd	Vol	Page	217
BIP from old book - Page No- 31 date, 29/3/09 8/10/11 ✓ 15/4/13 ✓	2	3	3	
46/9/14 Rel from store MSR P. no. 256 Donated by rotary club. Telling 403A as 2980 ✓	1	1	4	
13/11/18 (LP) Rd from store (Safe Touch) Transfer LP Books (P 203)	1		5	
26/2/19 (LP) Rd from store (anti Compressing) B. Gard	1		6	
24/9/19 Conded AS per order of THCAH varla. order no. W/2 1285/19 dated 24/9/19 (29/3/09 D, 8/10/11, 15/4/13) 1 (vol. ~)		3	3	✓
29/4/2023 Rel from store nebrulizer Recd Bro NE 0003 as NO 22090885 (P 1388) BARCODE 0552436	1		3	
2/6/2023 PUT IN VUG (Rid on 24/4/23)		1		NOT WORKING