

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THRISSUR
2	Name of Hospital	CHC VALAPAD
3	Name of Equipment with Make, Model and Serial Number	Centrifuge Make : REMI Model: R4C SN:LELC12G27
4	Equipment ID/ Barcode	0831056 #102492
5	Date of purchase/ Year of manufacture/Installation Date	06-06-2012
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free- 21-03-24
9	Action taken	Checked the machine and Found electric motor, knob for speed regulator and transformer defective. Need to replace these spares for further checking.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	Electric motor -6443/- Knob for speed regulator -58/- Transformer -971/- Total -7472/-

13	Asset Value	10316 /-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	72.43%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Service report and quotation attached
16	Reasons for recommending the equipment as BER	Checked the machine and found electric motor, knob for speed regulator and transformer are defective . Equipment installed on 06-06-2012 aged up to 13 years 8 month. Service quotation attached. service charge is 72.43% of asset value. So as per tender clause 5.3.14.1 the equipment recommending for condemnation.
17	Name & Signature of CYRIX Authority	BIJO T JOY

*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

spare cost not cost effective

Junior Consultant (Biomedical)
NHM, Thrissur

[Handwritten Signature]

Signature of JC BM (NHM)



SUPERINTENDENT
COMMUNITY HEALTH CENTRE
VALAPAD

[Handwritten Signature]

Signature of
Superintendent/Medical Officer (i/c)

Date: 18/4/24 -



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 193435

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility : <i>CHC</i>	Call Registration Date : <i>21/03/24</i>
Address : <i>VALAPAD</i>	Caller ID : <i>102492</i>
<i>THRISSUR</i>	Date of Visit : <i>22/03/24</i>
Ph : <i>9846752246</i>	Asset No. : <i>0831056</i>
	EQPT Name : <i>CENTRIFUGE</i>
	Manufacture : <i>REM1</i> Model : <i>R4C</i>
	S. No. : <i>WELC12927</i> Dept. : <i>LMB</i>

Service Classification : Breakdown Call **PMS** **Calibration** **Cust.Training**

Problem Identified : *MACHINE NOT SWITCHING ON*

Action Taken : *CHECKED THE MACHINE & FOUND ELECTRIC MOTOR, COILS FOR SPEED REGULATOR & TRANSFORMER DEFECTIVE . NEED TO REPLACE THESE SPARES FOR FURTHER CHECKING*


Completed **Date :** *22/03/24* **Time :** *11:00 AM* **Spare Required**

Spare Replaced **Requested**

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<i>AMBADY VS</i>	<i>22/03/24</i>	<i>10:00 AM</i>	<i>11:00 AM</i>

Customer Remark **Completed**

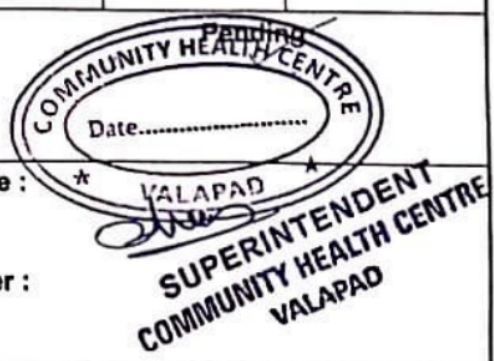

Service Engineer Name : *AMBADY VS*
Signature : *[Signature]*
Date : *22/03/24*
Contact Number : *7907996506*

Customer Name :
Signature :
Date :
Contact Number :
Designation :
Hospital Seal :

REMI SALES & ENGINEERING LIMITED

70/1750,5th Cross Road , Link Park ,Pottakuzhi Road, Pachalam P.O, Kochi-682012
 Phone : 0484-2401361,Email Id.:instservicekochi@remigroup.com/service@remilabworld.com

Corporate Off : Remi House, 3rd floor, 11 Cama Indl. Estate, Goregaon (East) Mumbai 400 063. INDIA
 • Board: +91 22 4058 9888 SALES SUPPORT NO.8879448682 • Email Id.: sales@remilabworld.com

QUOTATION CUM PROFORMA INVOICE

QN :6

Complaint No.	Customer Name & Address.:					Quotation No	PRINTED			
Dated	16/4/2024	CHC VALAPAD					Date	16/4/2024		
ENGINEER NAME	Vipin	DISTRICT INCHARGE THRISSUR					REF	Phone		
REF.	Phone	8921870010					DATE	16/4/2024		
Email	bijocyrix@gmail.com	BUO T JOY								
Model no.	R-4C	SR NO. /MFG DT.								
Sr No.	Description	Part code	HSN/SAC	Rate Rs.	Qty	Amount Rs. (A)	GST % (B)	GST Amt (C)	Total Amt (A+C)	
1	ELECTRIC MOTOR (RT	ML25000140	8501040	5460	1	5460	18%	983	6443	
2	KNOB FOR SPEED REGULATOR (NRT)	L22000116	392390	49	1	49	18%	9	58	
3	TRANSFORMER(NRT)	L22000019	850490	823	1	823	18%	148	971	
								TOTAL (D)	7472	
CALIBRATION CHARGES		0	0	0	0	0	0	0	0	
SERVICE CHARGES		0	0	0	0	0	18%	0	0	
								TOTAL (E)	7472	
Rupees in Words:		Rs. Seven thousand four hundred seventy two only .								7472

Terms & Conditions:

- Spares are suitable only to use with REMI instruments & not for any other make.
- We will accept return of spares only if they are unused and not damage. At our discretion, the returned spare will be replaced. The difference in prices. If any will have to be borne by you.
- To ensure supply of correct spares, we suggest you to send us defective spare in advance with your request for which you want to purchase new spares.
- 100 % Advance along with your order confirmation
- Payment can be made by Cheque/ NEFT in our Bank account. For Cash Payment you must collect Receipt from recipient of cash failing which REMI will not be held responsible for any discrepancy.
- Courier/ transportation charges are payable at destination & not included in our price.
- Validity. The quotation is valid for 30 days from the date of this quotation / Proforma Invoice
- Subject to Ernakulam Jurisdiction only

REMARKS : PAYMENT 100% ADVANCE

For REMI SALES & ENGINEERING LTD



BANK DETAILS FOR REMI SALES & ENGINEERING LTD.

- A/C NO: 35699154671
- IFS CODE: SBIN0013223
- GST NO: 32AAACR0421M12S
- Bank Name: STATE BANK OF INDIA
- MICR CODE:682002053
- PAN NO: AAACR0421M
- BRANCH: ELAMAJKARA
- SWIFT CODE: SBININBB395
- CIN NO. U31100MH198PL022314





RE: Re: CHC VALAPAD - 0831056 - 102492 - FOR QUOTATION

1 message

instservicekochi <instservicekochi@remigroup.com>

Tue, 16 Apr, 2024 at 12:02 pm

To: bijocyrix@gmail.com

Cc: Raman <raman@remilabworld.com>, REMI Group - Kochi - Vishnu S K <kochisales.hcd@remigroup.com>, kochi@remigroup.com

Dear Sir,

Please find the attached PERFORMA INVOICE for your reference. **PLEASE RELEASE THE PAYMENT IN ADVANCE.**

Regards

REMI KOCHI

INST DIV.

From: kochisales.hcd@remigroup.com <kochisales.hcd@remigroup.com>

Sent: Tuesday, April 16, 2024 10:39 AM

To: instservicekochi@remigroup.com

Subject: Fw: Re: CHC VALAPAD - 0831056 - 102492 - FOR QUOTATION

Rabiths

Please send quote

From: bijocyrix@gmail.com

Sent: Tue, 16 Apr 2024 09:22:57

To: kochisales.hcd@remigroup.com

Cc: Blesson Jose <zm2.klbemp@cyrix.in>, Sarang KM <sarangcyrix@gmail.com>

Subject: Re: CHC VALAPAD - 0831056 - 102492 - FOR QUOTATION

CAUTION: This email is from an external source. Exercise caution when opening attachments or clicking links.

Kindly provide the quotation

On Fri, 12 Apr, 2024, 7:21 am Bijo T Joy, <bijocyrix@gmail.com> wrote:

Reminder

On Tue, 9 Apr, 2024, 1:34 pm Sarang KM, <sarangcyrix@gmail.com> wrote:

Dear sir

Kindly share the quotation as soon as possible

On Mon, Apr 8, 2024 at 8:22 AM Bijo T Joy <bijocyrix@gmail.com> wrote:

Reminder

On Tue, 2 Apr, 2024, 11:09 am Bijo T Joy, <bijocyrix@gmail.com> wrote:

Dear sir,

There is a complaint reported from CHC VALAPAD. Regarding the complaint with centrifuge remi R4c. Please share the price and availability of below mentioned spare parts as soon as possible.

equipment - centrifuge

make - Remi

model - R4C

hospital

name - CHC

Valapad

barcode -

0831056

ticket id -

102492

quotation

for - motor,

speed

regulator

and

transformer

With Regards,

BIJO T JOY

DISTRICT INCHARGE THRISSUR,

CYRIX HEALTHCARE PRIVATE LIMITED

30/641 B, Petta Junction | Poonithura | Kochi | Kerala-682038 Branches: Kerala | Karnataka || Tamil Nadu || Uttar Pradesh | Kuwait | Saudi Arabia
M:-8921870010 | E:- bijocyrix@gmail.com | W:- www.cyrixhealthcare.com | "

-

Thanks & Regards

Sarang.k.m

Divisional Incharge|**North Zone**

Bemp-Kerala

Mobile : **+91 7593847150**

Email : sarangcyrix@gmail.com

CYRIX HEALTHCARE (P) LTD

30/641B | Petta | Punithura | Kochi | Kerala- 682038

www.cyrixhealthcare.com

P

Save Environment, Please do not print this e-mail unless it's essential

- 1. BALANCE CENTRIFUGE TUBES
- 2. ENSURE USE OF RUBBER CUSHIONS FOR GLASS TUBES
- 3. BRING SPEED KNOB TO "OFF" AND INCREASE SPEED GRADUALLY
- 4. CHECK CARBON BRUSHES PERIODICALLY
- 5. CHECK GLASS FIT FOR NON WORKING OF JNT

R-4C LABORATORY CENTRIFUGE

REMI

MIN   RPM  



6888

Preventive Maintenance Schedule KCP

Q1 09/08/2022

Q2

CYRIX HEALTH CARE PVT LTD
BEMP SERVICE PROVIDER
PREVENTIVE MAINTENANCE SERVICE

FMS DONE ON

NEXT FMS DUE

PERFORMED BY

CYRIX MEDICAL EQUIPMENT MAINTENANCE PROGRAMS (INDIA)
TOLL FREE NO: 1800 - 425-7689

BAR CODE - (8004-08015228)
0831056

CYRIX

Cyrix Health Care Pvt Ltd
BEMP Service Provider
Preventive Maintenance Service
Call: 1800-425-7689
www.cyrixindia.com

