


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

<b>Sl. No</b>	<b>Particulars</b>	<b>Details</b>
1	Name of District	PALAKKAD
2	Name of Hospital	CHC KOPPAM
3	Name of Equipment with Make, Model and Serial Number	BP APPARATUS MAKE : OMRON MODEL : NA SN : NA
4	Equipment ID/ Barcode	0951196 #109271
5	Date of purchase/ Year of manufacture/Installation Date	05/10/2020
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	03/05/2024 (toll free)
9	Action taken	Checked the machine found not getting on. Problem with board , Display and air pump. Need to replace board , Display and air pump for further checking.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	RS.2200/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found not working. Problem with main board , display and air pump. Equipment installed on 05/10/2020. aged upto 3 year 7 months. Quotation not submitted since spare parts are not available on market. So we are recommended the equipment for condemnation
17	Name & Signature of CYRIX Authority	AKHILESH P 

\*Not mandatory

#Based on the period of life and value as per the BER guidelines

\* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Machine aged up to 3 years. Quotation not submitted.

Consultant (Biomedical Engg)  
NHM (Arogyakeralam), Palakkad




10/5/24

Signature of JC BM (NHM)

Date:



  
SUPERINTENDENT MEDICAL OFFICER  
KOPPAM, PULASSERY P.O.  
PALAKKAD DT.-679 307



**BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAMME  
UNDER  
NATIONAL HEALTH MISSION**



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

**CYRIX**  
HEALTHCARE PVT LTD

**No. :** 179084

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <u>CHC KOPPAM</u>	Call Registration Date : <u>2/05/24</u>
Address <u>Palakkad.</u>	Caller ID : <u>109271</u>
Ph : <u>9496617127</u>	Date of Visit : <u>4/5/24</u>
	Asset No. : <u>0951196</u>
	EQPT Name : <u>BP. APPARATUS</u>
	Manufacture <u>OMRON</u> Model : <u>NA</u>
	S. No. <u>NA</u> Dept. <u>OP</u>

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** not working

**Action Taken :** checked the machine found not getting on. Problem with board display and air pump. need to replace board, display and air pump for further checking


Completed  Date : 4/5/24 Time : 11:00 AM Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Tyja</u>	<u>4/5/24</u>	<u>10:00 AM</u>	<u>11:00 AM</u>

**Customer Remark**  Completed  **PENDING OFFICER**  
COMMUNITY HEALTH CENTRE  
KOPPAM, PULASSERY P.O  
PALAKKAD DT: 679 307



<b>Service Engineer Name :</b> <u>Tyja</u> <b>Signature :</b> <u>[Signature]</u> <b>Date :</b> <u>4/5/24</u> <b>Contact Number :</b> <u>88218098192</u>	<b>Customer Name :</b> <u>Mrs. H. Koppam</u> <b>Signature :</b> <u>[Signature]</u> <b>Date :</b> <u>4/5/24</u> <b>Contact Number :</b> <u>9496617127</u> <b>Designation :</b> <b>Hospital Seal :</b>
--	---




# BP APPARATUS

	Rel	Issd	Balance	Part
5/10/2020	Rel from store	1	1	} used in our office
5/10/2020	part in use (Automatic)		1	
24/5/2021	Rel from the store (Manual - Mercuryless)	1	2	
24/5/21	Pt is to use		2	



COMMUNITY HEALTH  
 KOPPAM, PULASSE.  
 PALAKKAD DT.-679 307



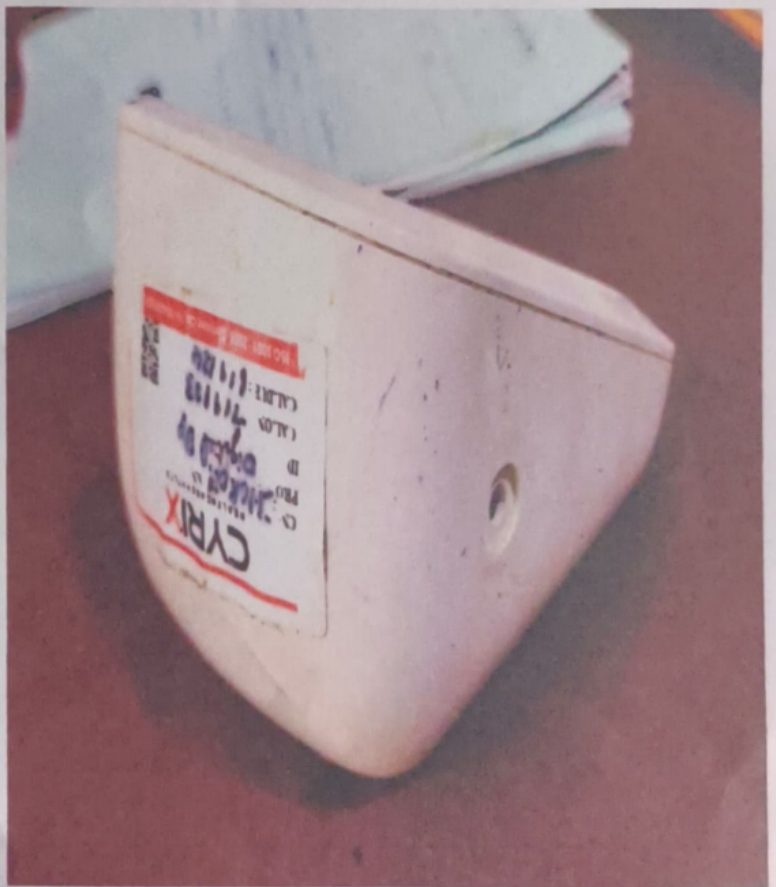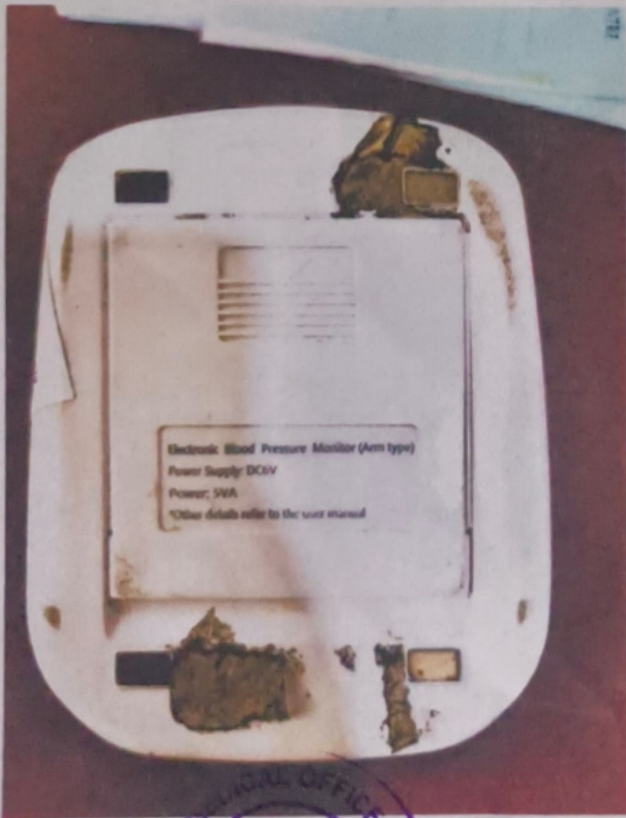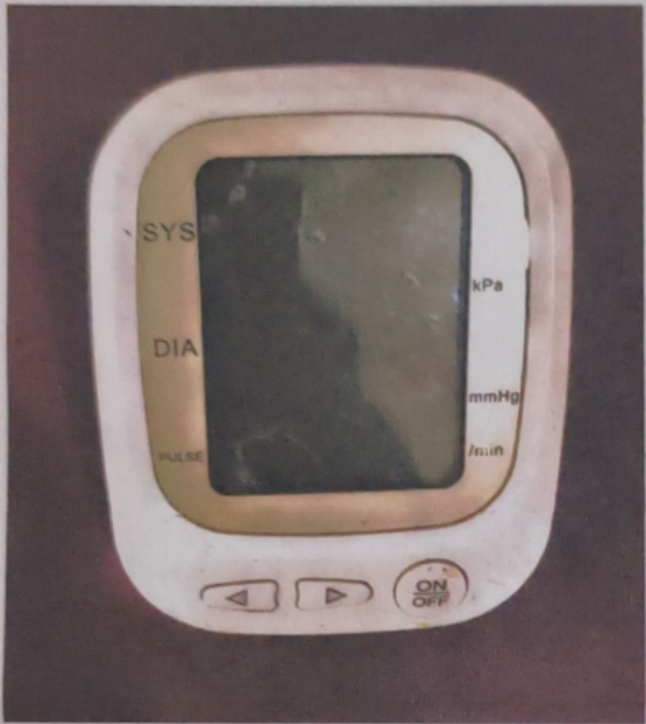

*my*  
COMMUNITY HEALTH CENTRE  
KOPPAM, PULASSERY P.O.  
PALAKKAD DT-679 307