


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KANNUR
2	Name of Hospital	PHC KODIYERI
3	Name of Equipment with Make, Model and Serial Number	WEIGHING MACHINE Make : SAMSO Model: NA SN:N/A
4	Equipment ID/ Barcode	1345029 #111409
5	Date of purchase/ Year of manufacture/Installation Date	10-03-2019
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free- 16-05-2024
9	Action taken	Checked the machine and found that Machine is not switching on, Found mainboard, Load cells damaged. Need to replace the these spares for further checking .
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA


13	Asset Value	1800 /-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Service report attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that machine is not switching ON. Found that main board and load cells damaged. Equipment installed on 10-03-2019. aged up to 5 years 2 months. Quotation not submitted since Spare parts are not available on market. So we recommend the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AVINASH T 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

checked & ident find that machine not switching on. Main board & load cells are damaged. Aged up to 5 years above. So its service cost economically not feasible. Recommended for BER as per BER Protocol.



25/05/2024

Signature of JC BM (NHM)

CONSULTANT BIOMEDICAL
NATIONAL HEALTH MISSION
KANNUR - 670002



Date: 27/5/2024


Dr Anurag
21/5/24

Signature of
Superintendent/Medical Officer (i/c)

പ്രാഥമികാരോഗ്യ കേന്ദ്രം
മുഴിക്കരയിൽ കേന്ദ്രം - കോട്ടിയേര
പി.ഒ മുഴിക്കര, കണ്ണൂർ - 670 103
ഫോൺ 0490 2356102



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 217010

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility PHC KODIYERI</p> <p>Address KODIYERI</p> <p style="padding-left: 100px;">KANNUR</p> <p>Ph : 09947506283</p>	<p>Call Registration Date : 16/05/2024</p> <p>Caller ID : 111409</p> <p>Date of Visit : 17/05/2024</p> <p>Asset No. : 1345029</p> <p>EQPT Name : WEIGHING MACHINE</p> <p>Manufacture SAMSUNG Model : NA</p> <p>S. No. NA Dept. OP</p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Machine is not switching ON

Action Taken : checked the machine and found that machine is not switching ON, found mainboard, Load cells damaged. Need to replace the these spares for further checking

Completed Date : 17/05/2024 Time : 1:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			



Cyrix Engineer	Date	Start Time	End Time
Prathyush T. Bhaskar	17/05/2024	12:30pm	1:00pm

Customer Remark Completed Pending

Service Engineer Name : Prathyush T. Bhaskar
Signature : *[Signature]*
Date : 17/05/2024
Contact Number : 9947025643



Customer Name : Venu m
Signature : *[Signature]*
Date : 17/05/24
Contact Number : 828194
Designation : Nursing office Gr I
Hospital Seal : *[Seal]*

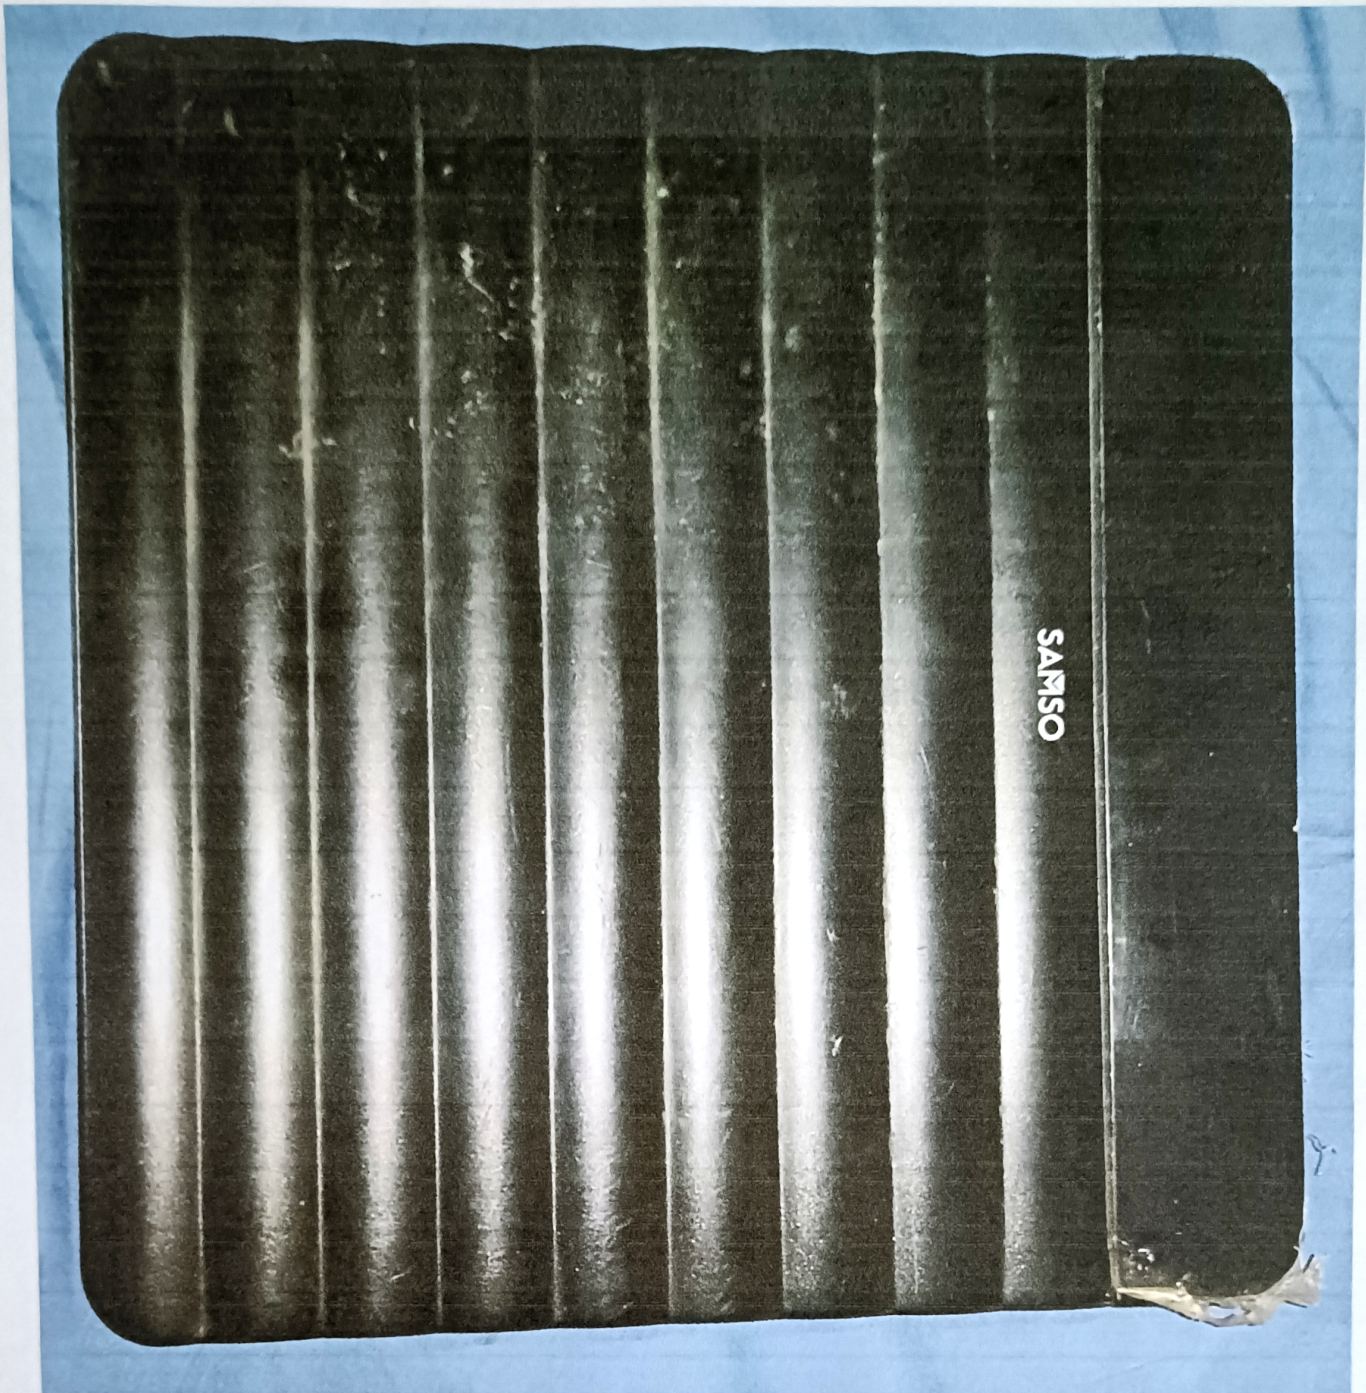

Handwritten notes in Malayalam and English. The text includes: 'പ്രോജക്ട് നമ്പർ = 870 103' (Project number = 870 103), 'പോസ്റ്റ് നമ്പർ 2356183' (Post number 2356183), and 'കോഴിക്കോട്' (Kozhikode). There is also a signature and a date '2023'.