



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 193966

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <i>THQH, Kayamkulam</i>	Call Registration Date : <i>21/03/2024</i>
Address <i>Allepuzha</i>	Caller ID : <i>102562</i>
<i>Kerala</i>	Date of Visit : <i>22/03/2024</i>
Ph : <i>8606817608</i>	Asset No. : <i>0421040</i>
	EQPT Name : <i>ECG Machine</i>
	Manufacture <i>BPL</i> Model : <i>Cardiac 6108T</i>
	S. No. <i>AVMP3G-22058</i> Dept. <i>ECG Room</i>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : *Not getting ON*

Action Taken : *Checked the machine and Found that the ECG Main PCB, Battery and printer Head Assembly are defective. Enquired the OEM for spares. Need to replace these spares for further checking and working condition of the equipment.*

Completed Date : *22/3/24* Time : *2:00 pm* Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<i>Mardula G</i>	<i>22/03/24</i>	<i>12:30 pm</i>	<i>2:00 pm</i>

Customer Remark Completed Pending

Service Engineer Name : <i>Mardula G</i>	Customer Name : <i>Chinchi.v</i>
Signature : <i>Mardula G</i>	Signature : <i>Chinchi.v</i>
Date : <i>22/03/2024</i>	Date : <i>22/03/24</i>
Contact Number : <i>9081199471</i>	Contact Number : <i>8606817608</i>
	Designation : <i>ECG Technician</i>
	Hospital Seal :



7
Govt. Taluk Hospital
Kayamkulam



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 193916

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility <u>THQH, Kayamkulam</u>	Call Registration Date : <u>21/03/2024</u>
Address <u>Alappuzha</u>	Caller ID : <u>102562</u>
<u>Kerala</u>	Date of Visit : <u>22/03/2024</u>
Ph : <u>8606817608</u>	Asset No. : <u>0421040</u>
	EQPT Name : <u>ECG Machine</u>
	Manufacture <u>BPL</u> Model : <u>cardiac 6108T</u>
	S. No. <u>AVMP3G20058</u> Dept. <u>ECG Room</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not getting ON

Action Taken : checked the machine and found that the ECG Main PCB, Battery and printer Head Assembly are defective. Enquired the OEM for spares.

Completed Date : 05/04/24 Time : 1:30 PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Mridula G</u>	<u>05/4/24</u>	<u>12:45 PM</u>	<u>1:30 PM</u>

Customer Remark Completed Pending
Requesting for confirmation chupcheru
chinch 5/04/24

Service Engineer Name : <u>Mridula G</u>	Customer Name :
Signature : <u>[Signature]</u>	Signature :
Date : <u>05/04/2024</u>	Date :
Contact Number : <u>9061199471</u>	Contact Number :
	Designation : <u>Superintendent</u>
	Hospital Seal : <u>Govt Taluk Hospital Kayamkulam</u>




**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	ALAPPUZHA
2	Name of Hospital	THQHKAYAMKULAM
3	Name of Equipment with Make, Model and Serial Number	ECGMACHINE MAKE :- BPL MODEL:-CARDIART6108T SN :- AVMP3G22058
4	Equipment ID& Barcode	102562&0421040
5	Date of purchase/Year of manufacture /Installation Date	31/08/2013
6	Warranty details(Yes/No)	NOWARRANTY
7	*AMC/CAMC Period agreed at the time Of purchase	NOAMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	21/03/2024
9	Action taken	Checked the machine and found that the ECG Main PCB, Battery & Printer Head Assembly are defective. Enquired the OEM for spares.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not Recommending for repair
12	Cost of spares(specify parts and cost)	Main PCB Assay 6108 T :-14000/- NIMH Battery 9.6V , 1.4Ah :- 2048/- <u>PrintHeadAssembly6108T:-2206.6/-</u> Total :-18254.6/-


13	Asset Value	RS:- 23391.38/-
14	#Percentage value of the cost of spares with respect to Cost of Purchase/Asset Value	78%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service Report & OEM Quotation Attached.
16	Reasons for recommending the equipment as BER	Checked the machine and found that the ECG Main board, Battery & Printer Head Assembly are defective. Enquired the OEM for Quotation. This equipment installed on 31/08/2013, aged upto 10 years and 7 months. Percentage of service cost is high (78%) and economically not viable. Both criteria met as per the tender clause 5.3.14.1 we are Recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	 MRIDULAG

*Not mandatory #Based on the period of life and value as per the BER guidelines

*Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical)NHM:

Recommended for BER



JYOTHISH THOMAS
 Consultant (Biomedical Engineering)
 NHM ALAPPUZA
 Signatory of JCBM(NHM)

Signature for Condemnation

Date



Seal


 Signature of Superintendent/Medical Officer (i/c)

Superintendent
 Govt. Taluk Hospital
 Kayamkulam

ECG MACHINE

B/F page 13 3183
 24.12.05 IN. No. 293/05-06 Dms Alappally machines 05080796 issued
 Rs. 12500/each 1 1 Nil

22.2.06 issued to ECG Technician 1 Nil

- Power cord 3pin - 1
- Patient Cable (10 lead lead type) - 2
- Clamp electrodes - 1 set
- Chest Electrodes with Bullans - 6 Nos
- ECG Jelly bottle - 2 Nos
- Earthing Cable - 1 no
- paper Roll 55mm - 1 no
- User's manual - 1
- Warranty card - 1
- Baluru Nil

5/6/13 W.No: CAM/FG/98/13-14 dttd 31.05.2013 from BPL Limited
 No. 35-261, Milma dairy, Meethanar Road, Koonamthai, Edappally, Cochin

BPL ECG MODEL 61087 (1) 23,450.00 (1)
 one pmt tax - VAT @ 5% 1172.50
24,622.50

Issued to ECG Technician 1 Nil
 Baluru Nil

Received
 Shreejith

21.8.2013 W.No: EKM/FG/203/13-14 dttd 29/Aug/2013 from BPL Ltd No: 35-261
 Milma dairy - Meethanar Road, Koonamthai, Edappally, Cochin



1. BPL ECG MODEL 61087 (1) 22,277.50
 one pmt tax - VAT @ 5% 1113.88


Issued to ECG Technician 1 23,391.38
 Baluru Nil

Received
 Shreejith
 P. G. T. K.

C/O to 134

Superintendent
 Govt. Taluk Hospital
 Kayamkulam

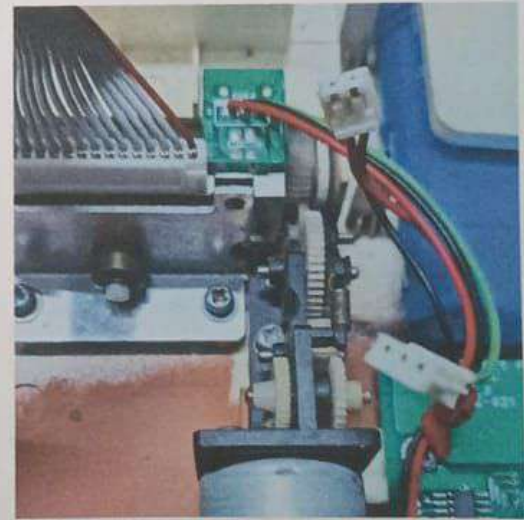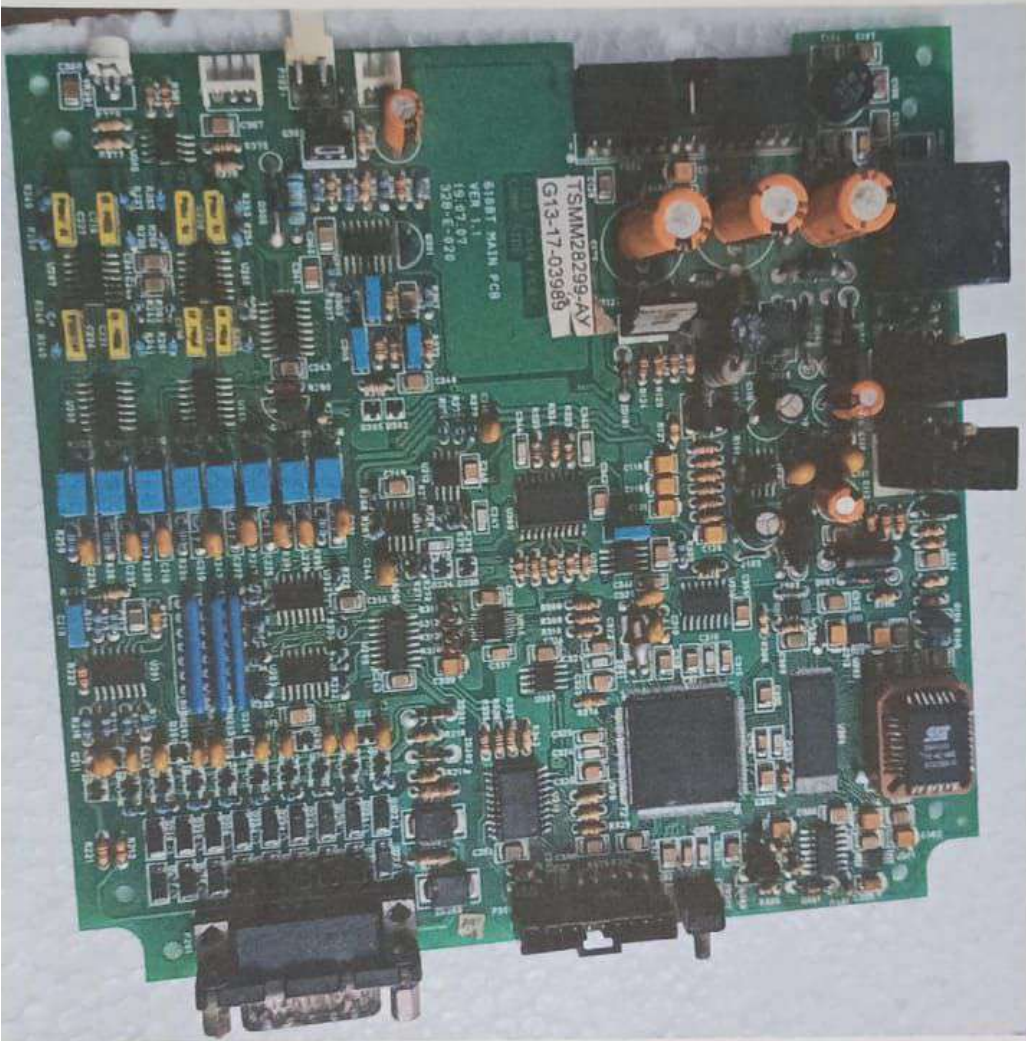


 Superintendent
 Govt. Taluk Hospital
 Kayamkulam



QTN/BISO/050424-002

05/04/2024

QUOTATION

To,
CYRIX HEALTH CARE PVT LTD
ERNAKULAM

Dear Sir,

Please find below our lowest quotation for the following items:-

SL NO.	ITEM DESCRIPTION	COST PER UNIT	UNIT PRICE
1	ECG 6108T MAIN PCB ASSY NEW (WITH LPC IC)	12500	12500+12%TAX
2	BM/OM NIMH BATTERY 9.6V 1.4 AH	1600	1600+28%TAX
3	PRINT HEAD ASSY 6108T	1870	1870+18%TAX

Terms and conditions:

1. Payment 100% in advance along with Purchase order
2. Delivery within 15 days

Thanking you and assuring you our best attention always.

For Biomedix Solutions



Authorized Signatory

Mobile: 9846969564 | Email: biomedixservice@gmail.com

Branches: Kozhikode, Kannur, Kottayam-Kollam.

For enquiries contact: biomedixsales@gmail.com, biomedixservice@gmail.com



BIOMEDIX SOLUTIONS

No: 7/437- B, Mannarakayam P.O,
Kathilankalpadi, Kanjirapally, Kottayam - 686506,
Mob:9846969564,