



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 196476

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.y@cyrix.in

| | | | |
|-----------------|----------------|--------------------------|-------------------------|
| Health Facility | CHC Malippuram | Call Registration Date : | 24-02-2024 |
| Address | Ernakulam | Caller ID : | 98010 |
| | Ernakulam (Dt) | Date of Visit : | 26-02-2024 |
| Ph : | 9446366945 | Asset No. : | 0731113 |
| | | EQPT Name : | BP Apparatus |
| | | Manufacture | OMRON Model : HEM-7620 |
| | | S. No | 20170515851671 Dept. OP |

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : BP Apparatus not working

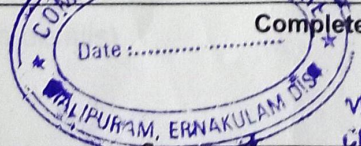
Action Taken : checked the machine and found that pressure sensor and control board are defective.



Completed Date : 26-02-24 Time : 10:30AM Spare Required

Spare Replaced Requested

| Description | Qty. | Part Number | PR Number |
|--------------------|-------|-------------|-----------|
| 1. Pressure Sensor | 1 No. | | |
| 2. Control Board | 1 No. | | |
| 3. | | | |

| Cyrix Engineer | Date | Start Time | End Time |
|---------------------|----------|------------|----------|
| Jibin Thomas George | 26-02-24 | 9:00AM | 10:30AM |

Customer Remark :  Completed for Pending


| | |
|---|--|
| Service Engineer Name : Jibin Thomas | Customer Name : Shini C.K |
| Signature :  | Signature :  |
| Date : 26-02-2024 | Date : 26/2/24 |
| Contact Number : 9047958051 | Contact Number : 9446366945 |
| | Hospital Seal : Senior nursing officer |

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

| Sl. No | Particulars | Details |
|--------|---|--|
| 1 | Name of District | Ernakulam |
| 2 | Name of Hospital | CHC MALIPPURAM |
| 3 | Name of Equipment with Make, Model and Serial Number | BP Apparatus Make : OMRON Model : HEM-7120 Sr.no-: 20170515851VG1 |
| 4 | Equipment ID & Barcode | 0731113 & 98010 |
| 5 | Date of purchase / Year of manufacture /Installation Date | 30/10/2019 |
| 6 | Warranty details (Yes/No) | No warranty |
| 7 | *AMC/ CAMC Period agreed at the time of purchase | No AMC/CAMC |
| 8 | Date of breakdown(Date of registration of complaint through email/ Toll free) | 24-02-2024 |
| 9 | Action taken | Checked the machine and found that pressure sensor and control board are faulty. |
| 10 | Present status of the equipment (Fully damaged / partially damaged) | Fully damaged |
| 11 | Recommendations for repair (required service details) | It is not recommend for repair |
| 12 | Cost of spares (specify parts and cost) | NA |

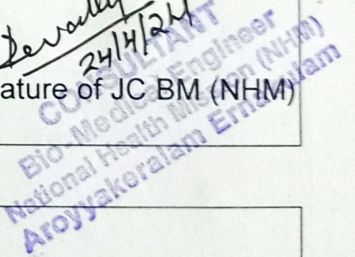
| | | |
|----|--|---|
| 13 | Asset Value | RS.2,200 |
| 14 | # Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value | NA |
| 15 | Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) | Cyrix service report attached |
| 16 | Reasons for recommending the equipment as BER | Checked and found pressure sensor and control board are defective. Equipment installed on 30-10-2019 and outlived 4+years. Quotation not submitted since the spares are not available in the market. So recommending the equipment for condemnation |
| 17 | Name & Signature of CYRIX Authority | JIBIN THOMAS GEORGE  |


*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Devally
24/4/24
Signature of JC BM (NHM)




Superintendent / Medical Officer (i/c)
MEDICAL OFFICER INCHARGE
COMMUNITY HEALTH CENTRE
MALIPURAM, ERNAKULAM

Signature of seal



Date

DIGITAL B.P. APPARATUS

30/10/19. Received from store.

(Omission HEM - 7(21J) - 7121J)

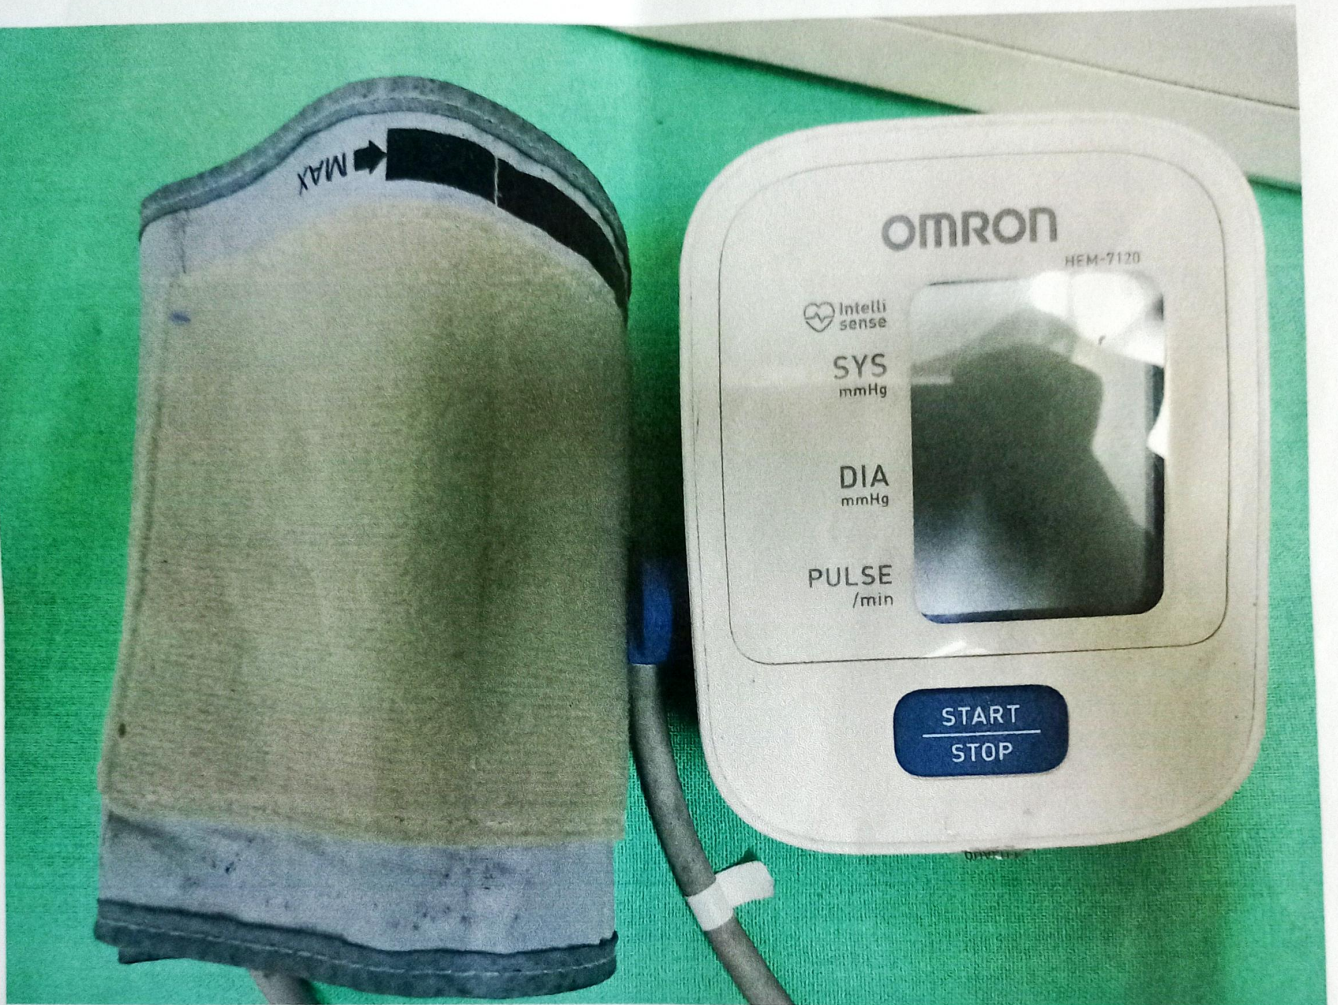
RA 1800x24 GST. invia no: CSA/
02026/19-20, Cochin Superck)

| RE | ISSUE | Date | SI |
|----|-------|------|-----|
| 2 | - | 2 | |
| 01 | | 03 | 1/1 |
| | 01 | 02 | |
| 01 | | 04 | 1/3 |

8/12/22 Received from the store
Invoice no: 1556 from K.C. Kunyia cost - 2350/-
(Digital Life line) issued to PHCI

3/8/22 Received from the store
Invoice no: 1556 from Kunyia
cost - 2350/- Digital life line.








OMRON

AUTOMATIC BLOOD PRESSURE MONITOR

MODEL : HEM-7120

RATING : DC 6V 4W



SERIAL No. :

20170515851V61

OMRON HEALTHCARE Co., Ltd.
Kyoto, JAPAN



OMRON HEALTHCARE EUROPE B.V.
Scorpius 33, 2132 LR Hoofddorp
THE NETHERLANDS

Asia Pacific HQ :
OMRON HEALTHCARE
SINGAPORE PTE LTD.

