



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :
205169

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>THQH</u></p> <p>Address <u>THQH Sasthamcotta</u> <u>KOLLAM</u></p> <p>Ph : <u>94 9673 7513</u></p>	<p>Call Registration Date : <u>20/04/2024</u> .</p> <p>Caller ID : <u>107260</u></p> <p>Date of Visit : <u>22/04/2024</u> .</p> <p>Asset No. : <u>0222321</u></p> <p>EQPT Name : <u>Nebuliser</u></p> <p>Manufacture <u>Life Care</u> Model : <u>CNB69022</u></p> <p>S. No. <u>LC.2219040</u> Dept. <u>MM ward</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Nebuliser not getting on.

Action Taken : checked the nebuliser found that the motor defective and piston damaged. need to replace these spares for further checking working condition of this equipment.

Completed Date : 22/04/24 Time : 12:20pm Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.				
3.				

Cyrux Engineer	Date	Start Time	End Time
<u>Diswarya Raj - k.n</u>			
<u>Dr. Anup S Nkbs, Dch</u>			

Customer Remark Removed defective part
Phone 36549
THQH Sasthamcotta

Completed Pending

Service Engineer Name Diswarya Raj

Signature : [Signature]

Date : 22/04/24

Contact Number : 9645384568

Customer Name : Manceesh M

Signature : [Signature]

Date : 22/4/24

Designation : Nursing officer

Hospital Seal : 9847161413




**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	Kollam
2	Name of Hospital	THQH SASTHAMKOTTA
3	Name of Equipment with Make, Model and Serial Number	NEBULIZER Make : Life care Model : CNB69022 SI no: LC2219040
4	Equipment ID & Barcode	Barcode : 0222321 / Ticket id : 107260
5	Date of purchase / Year of manufacture / Installation Date	28-09-2019
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	20-04-2024
9	Action taken	Checked the machine found that the Nebulizer motor and piston are damaged condition, Enquired spares in the market
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not Recommended for Repair
12	Cost of spares (specify parts and cost)	NA


13	Asset Value	Rs. 1353/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that the nebulizer motor and piston are defective, enquired for spares in the market but spare are not available. Equipment is installed on 28-09-2019 and aged up to 4 years and 6 months. So we are recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AISWARYA 

*Not mandatory #Based on the period of life and value as per the BER guidelines


* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Supai Fully damaged and recommended for Beyond economic


21.05.24
Signature of J. B. M. (NHM)
NHM, KOLLAM



Date



Seal



Signature of Superintendent /
SUPERINTENDENT
Taluk Head Quarters Hospital
Sasthamcotta

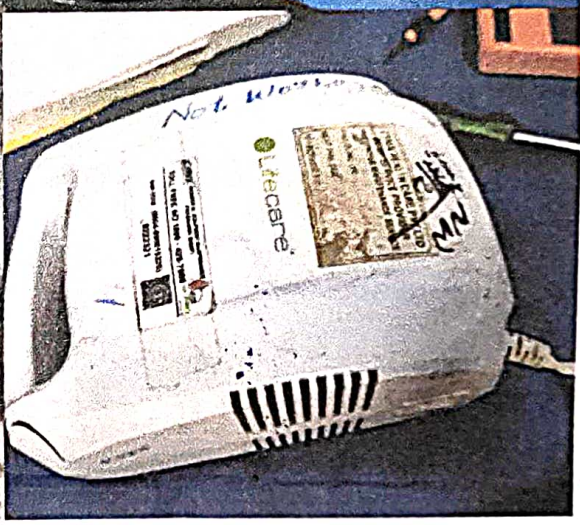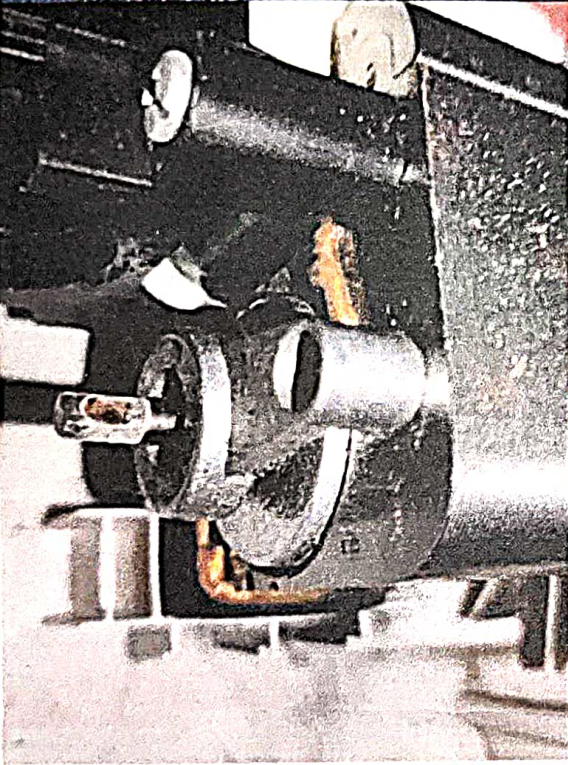


[Signature]
SUPERINTENDENT
Taluk Head Quarters Hospital
Sasthamcotta

Date	Name	Receipt	Issued	Balance	Remarks
05/12/2019	RECORDER B/E from Assistant State Engineer for I page no. 88			7	

16/11/20	electronic nos (3) @referred as per order no 1634/2020 dttd 16/11/20			4	
11/12/1	Recd from store	2		2.5	
20/11/20	Tr. out to covered land		1	5	
4/12/20	Tr. in from covered land (Page : 123 contd 121)	(1)		6	

BARCODE.

- (1) 0222 330.
- (2) 0222 321.
- (3) 0222 322.
- (4) 0222 328.
- (5) 0222 325.
- (6) 0222 327.


 Dr. Anand Kumar Das
 Puro Pakshacharya
 June 2019
 JSTH Sasthancotta
SUPERINTENDENT
 Taluk Head Quarters Hospital
 Sasthancotta