



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

# CYRIX

HEALTHCARE PVT LTD

**No. :** 220660

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : <u>GH</u></p> <p>Address : <u>General hospital</u> <u>Kottayam</u></p> <p>Ph : <u>80 755 35 967</u></p>	<p>Call Registration Date : <u>7/06/2024</u></p> <p>Caller ID : <u>115712</u></p> <p>Date of Visit : <u>10/06/2024</u></p> <p>Asset No. : <u>0510486</u></p> <p>EQPT Name : <u>BP Apparatus</u></p> <p>Manufacture <u>Yuwell</u> Model : <u>YE680A</u></p> <p>S. No. <u>20190601429</u> Dept. <u>NGD clinic</u></p>
--	---

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** BP Apparatus - digital not working  
main PCB and motor not working

**Action Taken :** Tried to repair and failed. Spare parts are  
not available in the market. Repairing is not  
possible.

Completed  Date : ..... Time : ..... Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Sarish Sivan</u>	<u>10/6/24</u>	<u>1:30pm</u>	<u>2:30pm</u>

Customer Remark  Completed  Pending

Equipment is not working need replacement

<p>Service Engineer Name: <u>Sarish Sivan</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>10/6/24</u></p> <p>Contact Number : <u>9946646571</u></p>	<p>Customer Name : _____</p> <p>Signature : _____</p> <p>Date : _____</p> <p>Contact Number : _____</p> <p>Designation : _____</p> <p>Hospital Seal : _____</p>
--	---




17/6/24


Superintendent i/c  
General Hospital  
Kottayam

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

Sl. No	Particulars	Details
1	Name of District	KOTTAYAM
2	Name of Hospital	GH KOTTAYAM
3	Name of Equipment with Make, Model and Serial Number	Equipment :BP APPARATUS Make: YUWELL Model :YE680A SN: ID2019041429
4	Equipment ID & Barcode	115712 & 0510486
5	Date of purchase / Year of manufacture /Installation Date	21/01/2020
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	07/06/2024 (Toll free) 
9	Action taken	Checked and found out the problem main PCB and NIBP pump
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	N/A


13	Asset Value	Rs. 1750/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found out the problem with main PCB and NIBP pump. Machine installed in 21/01/2020 and covered up to 4 + years. Quotation not submitted since spare are not available in the market. So recommended the machine for condemnation
17	Name & Signature of CYRIX Authority	Sanish sivan 

\*Not mandatory #Based on the period of life and value as per the BER guidelines

\* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Asset value - 1750  
 Cost of spare - Quotation not attached, mentioned as spare not available  
 Life period - 21/1/20 to 26/1/24 - 4 years  
 As per the BER guidelines recommended as Beyond repairable.

  
 Signature of JC BM (NHM) on 24/6/24

CONSULTANT ENGINEER  
 NATIONAL HEALTH ENGINEERING  
 KOTTAYAM

Date

  
 Seal

  
 Signature of Superintendent i/c General Hospital Kottayam  
 Superintendent Medical Officer (i/c)

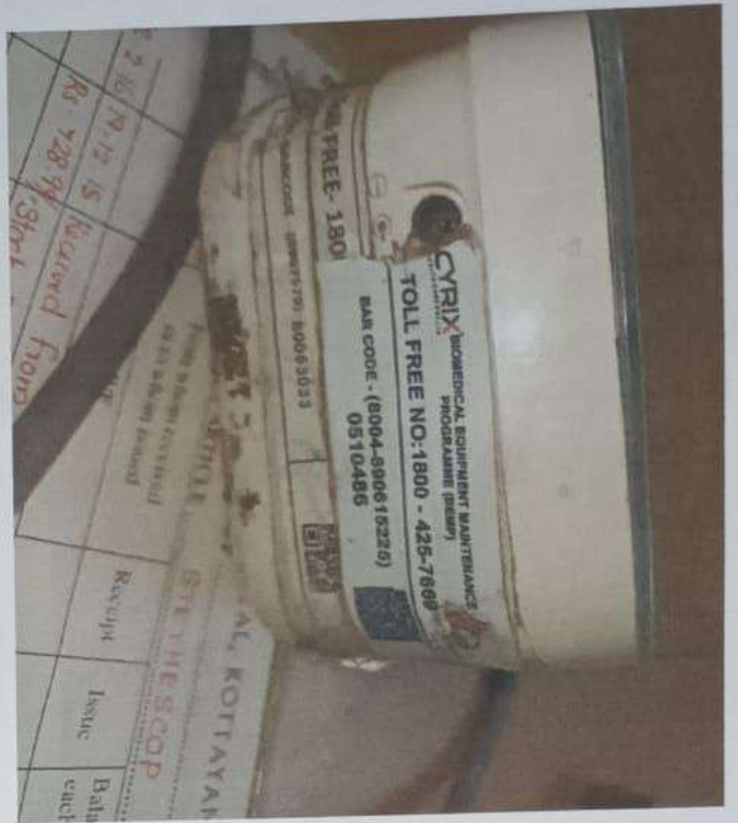
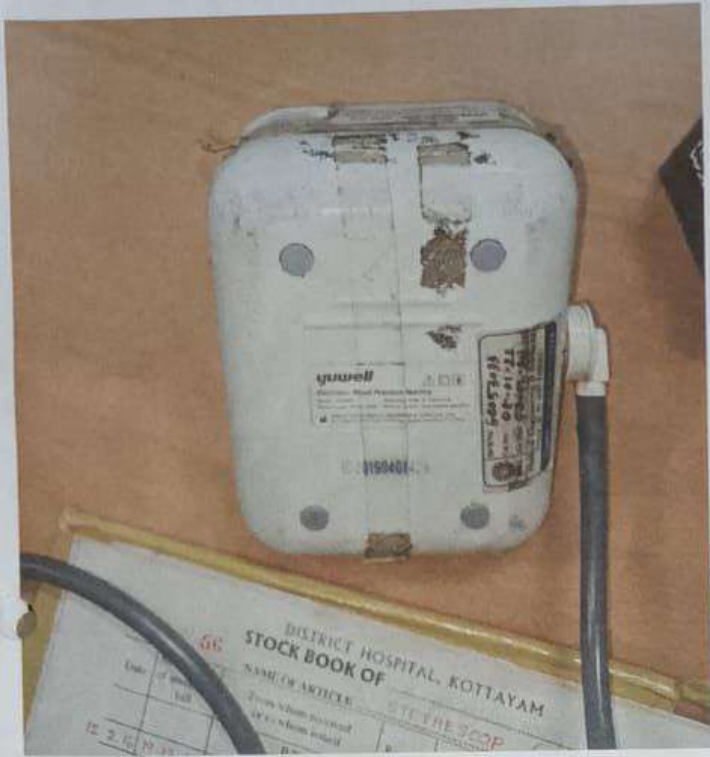
# DISTRICT HOSPITAL, KOTTAYAM STOCK BOOK OF .....

NAME OF ARTICLE B. P. APPARATUS 57 (NCD)

Date	No. and date of invoice or bill	From whom received or to whom issued	Receipt	Issue	Balance after each transaction	Initials of receiver	Remarks
		B/F					
12-2-16	19.12.15	Received from ELKO PPunit stock reg Regulator P: 172	1		1	<i>Dr. Dietician</i>	CYRIX BARCODE 0510483
12-2-16	Rs: 1995/-	Issued for use		1			
30-7-16	13626	Received from 30/7/16 PP Unit Stock Register Rs: 1650 P: 172	1		2	<i>Dr. Puthiyap</i>	0510485
30-7-16	(Kawanya CP Gift comp ound) Elko	Issued for use		1			
17-10-17	Diamond	Received from (Kawanya Store Stock Reg Pharmacy) (LP Vol: 23 p: no: 31)	1		3	<i>Dr. Dietician</i>	0510484
18-10-17	Rs: 2002/-	Issued for use		1			
3-1-19	KMBCL	Received from Store Digital Stock Reg p: 139	1		4	<i>Dr. Dietician</i>	
3-1-19		BPL 120/80 B5 Issued for use		1			
20-1-20	KL00503/ 00040/19-20	Received from store Digital BP Apparatus	1		5	<i>Dr. Puthiyap</i>	0510486
20-02-20		Issued for use		1			
10-3-2023		Received from Store (Digital BP Apparatus)	2	5			0510480
4/3/23		Issued for use Stock Register P: 118		2			0510481
		C/F					



27/1/23  
 J. S.  
 District Hospital  
 Kottayam



*JM*  
 Superintendent i/c  
 General Hospital  
 Kottayam

