



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

**No. :** 218990

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility ..... P.H. Eramallickara</p> <p>Address ..... Dist: Alappuzha</p> <p>Ph : ..... 854717426</p>	<p>Call Registration Date : 03/06/2024</p> <p>Caller ID : 114845</p> <p>Date of Visit : 04/06/2024</p> <p>Asset No. : 0441586</p> <p>EQPT Name : BP Apparatus</p> <p>Manufacture Elka Model : EL-5da</p> <p>S. No. 1851800303 Dept. OP</p>
--	--

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** Not getting on

**Action Taken :** Checks the machine and found that main board and battery holder are defective. Battery holder socket was rusted. Need to Replace These spare for further checking and working condition of the Equipment.


Completed  Date : 25/6/2024 Time : 2:30pm Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Saveth Chandran	25/6/2024	1:30pm	2:30pm
	"	"	"

**Customer Remark** Completed  Pending



**Service Engineer Name :** Saveth Chandran  
**Signature :** *Saveth*  
**Date :** 25/6/2024  
**Contact Number :** 8075052698

**Customer Name :** Beenaheman TK  
**Signature :** *Bees*  
**Date :** 25/6/2024  
**Contact Number :** 9447084450  
**Designation :** Medical Officer  
**Hospital Seal :** *Bees*  
MEDICAL OFFICER IN CHARGE  
PRIMARY HEALTH CENTRE

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

<b>Sl. No</b>	<b>Particulars</b>	<b>Details</b>
1	Name of District	ALAPPUZHA
2	Name of Hospital	PHC ERAMALLIKKARA
3	Name of Equipment with Make, Model and Serial Number	BP APPARATUS MERCURY FREE MAKE :- ELKO MODEL :- EL 520 SN :- 18051800303
4	Equipment ID & Barcode	114845 & 0441586
5	Date of purchase / Year of manufacture /Installation Date	21/01/2021
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	03/06/2024
9	Action taken	Check the machine and found that main board and battery holder are defective. Battery holder socket was rusted.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not Recommended For Repair
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	RS:- 1940/-
14	#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service Report Attached
16	Reasons for recommending the equipment as BER	Check the machine and found that main board and battery holder are defective. Battery holder socket was rusted condition. Equipment was installed on 21/01/2021 and aged up to 3 years and 4 months. Quotation is not submitted since spares are not available in the market. So we are recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	SARATH CHANDRAN <i>Sarath</i>

\*Not mandatory #Based on the period of life and value as per the BER guidelines

\* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

*Recommended for BER*

*[Signature]* 24/06/24  
 JYOTHISH THOMAS  
 Consultant (Biomedical Engineering)  
 ERAMALLIKKARA  
 Signature of JUC BM (NHM)


Date *25/6/2024*



*[Signature]*  
 Signature of  
 Superintendent / Medical Officer (J/C)  
 PRIMARY HEALTH CENTRE  
 ERAMALLIKKARA



BP Apparatus

		Received	Balance	Remark Initial
12/2/14	BF from page no: 9	1	1	[old Equipment Register] <del>1</del>
3/8/19	BP Apparatus mercury free	1	2	
22/8/18	Damaged in natural calamity. not usable. Entered in Register of unserviceable Article Page 2			
14/9/2018	MERCURY FREE BP APPARATUS FROM (W) STORO ALAPP IN NO 617/18-19 on 13/9/18. (Diamond)	1	1	
	Main stock Register of Equipment P.No.3.			
14/9/18	OMRON AUTOMATIC BLOOD PRESSURE MONITOR HEM7120 / OMRON HEM7120 CASE RATE 2340/-	1	2	Not working Note Nil Moved to unserviceable Article Register on
22/1/2020	MEDICARE PHARMASUTICALS CHEMICALS (BN III, 1940-62) (Cuff set Inflator & Valve. 3 Batteries.) CMEDIVISION) Rate Rs 200/-	1	3.	2 in OP 1 EMO.
	MS. Ry. P.No. 3.			
21/1/21	ELKO mercury free Sphygmomanometer LTD DIS play Model EL 520 Ssp Janu 2028 Unit Rate 1940RS/- (BF. MS p.No. 3)	1	4	3 IN OP 1 EMO

  
 DR. JUNIGAL  
 M. J.  
 15/6/2024

MEDICAL OFFICER IN CHARGE  
 PRIMARY HEALTH CENTRE  
 ERAMALLIKKARA

M. J.  
 M. J.  
 on 15/6/2024

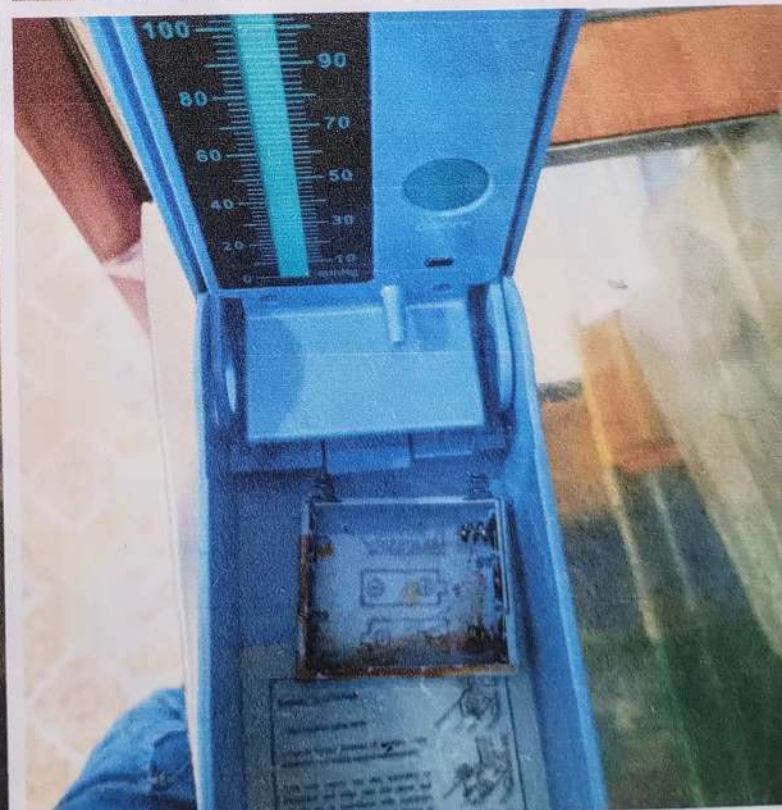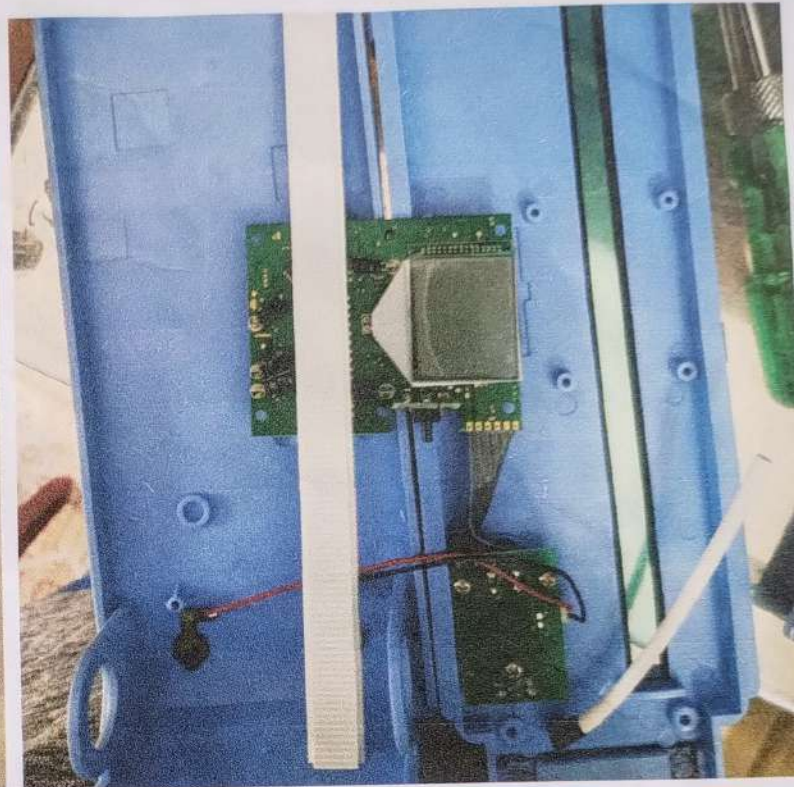

*S.V.*

MEDICAL OFFICER IN CHARGE  
PRIMARY HEALTH CENTRE  
ERAMALLIKKARA