


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	PALAKKAD
2	Name of Hospital	PHC OZHALAPATHY
3	Name of Equipment with Make, Model and Serial Number	WEIGHING MACHINE MAKE : OMRON MODEL : HN 283 SN : 201400353F1
4	Equipment ID/ Barcode	#91871 0941078
5	Date of purchase/ Year of manufacture/Installation Date	01/10/2018
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	20/01/2024 (toll free)
9	Action taken	Checked the machine found Load cells and Display damaged. Need to replace these spare for further checking.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	RS.3800/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found not working. Found Load cells and display defective. Equipment installed on 01/10/2018. aged up to 5 year 2 months. Quotation not submitted since spare are not available from market. So we are recommended the equipment for condemnation
17	Name & Signature of CYRIX Authority	AKHILESH P 


*Not mandatory

#Based on the period of life and value as per the BER guidelines


* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

checked and found that load cells and display damaged. hence recommended for BER.


Signature of (Biomedical Engg) Consultant (NHM), Palakkad
NHM (Arogyakeralam), Palakkad

Date: 12/4/24


Signature of "Superintendent/Medical Officer (i/c)"
12/4/2024 കേ.പ്ര.ഒ.
678 557

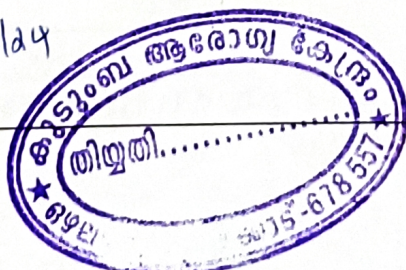



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 194418

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>PHC ozhalapathi</u></p> <p>Address <u>Palakkad</u> <u>Kerala</u></p> <p>Ph : <u>09544877578</u></p>	<p>Call Registration Date : <u>20-01-2024</u></p> <p>Caller ID : <u>91871</u></p> <p>Date of Visit : <u>22-01-2024</u></p> <p>Asset No. : <u>0941078</u></p> <p>EQPT Name : <u>weighing machine</u></p> <p>Manufacture <u>OMRON</u> Model : <u>HN-283</u></p> <p>S. No. <u>2014090353F</u> Dept. <u>OP</u></p>
---	--

Service Classification : Breakdown Call **PMS** **Calibration** **Cust.Training**

Problem Identified : unit not working

Action Taken : checked the machine Found lead cell and display damaged. need to replace these spares For Farther checking

Completed **Date :** 22-01-24 **Time :** 10:45 AM **Spare Required**

Spare Replaced **Requested**

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>ABIJITH - B</u>	<u>22-01-2024</u>	<u>10:30 AM</u>	<u>10:45 AM</u>

Customer Remark **Completed** **Pending**

<p>Service Engineer Name : <u>ABIJITH-B</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>22-01-2024</u></p> <p>Contact Number : <u>9567164651</u></p>	<p>Customer Name : <u>[Signature]</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>22/01/2024</u></p> <p>Contact Number : <u>9544877578</u></p> <p>Designation : <u>Nursing officer GRI</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
---	--



"മെഡിക്കൽ സർവീസുകൾ വാർത്ത"


[Handwritten notes and signatures]

OMRON
 DIGITAL BODY WEIGHT SCALE
 MODEL: HN-283 (HN-283-AP)
 WEIGHT DISPLAY: 5-150kg
 MINIMUM DISPLAY UNIT: 100g
 RATING: DC 3V 0.02W
 SERIAL NO.:

OMRON HEALTHCARE Co., Ltd. Kyoto, JAPAN
 MADE IN CHINA

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
 TOLL FREE NO: 1800 - 425-7669
 BAR CODE - (8004-890615225) 0941078

(414)67(254)09(21)5571



കുടുംബ ആരോഗ്യ കേന്ദ്രം
 തിരുതി.....
 ഔദ്യോഗിക, പാലക്കാട്-678557

[Handwritten Signature]
 "മെഡിക്കൽ ഓഫീസർ ഇൻ ചാർജ്ജ്"
 കുടുംബ ആരോഗ്യ കേന്ദ്രം
 ഔദ്യോഗിക, പാലക്കാട്-678 557

