


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	MALAPPURAM
2	Name of Hospital	PHC NANNAMBRA
3	Name of Equipment with Make, Model and Serial Number	Equipment: WEIGHING MACHINE Make: SAMSO Model: NA Serial Number : NA
4	Equipment ID/ Barcode	TICKET ID :115320 BARCORDE NO : 1041231
5	Date of purchase/ Year of manufacture/Installation Date	As per ticket master installation date: 20-10-2019 (As per stock book installation date is 30/08/2019)
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of Purchase	NO AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	05/06/2024
9	Action taken	Checked the machine and found problem board & display. Need to replace These spare for further checking
10	Present status of the equipment (Fully damaged / partially damaged)	NOT WORKING
11	Recommendations for repair (required service details)	No recommendation
12	Cost of spares (specify parts and cost)	N/A

13	Asset Value	1600/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX Service Report
16	Reasons for recommending the equipment as BER	Checked the machine and found board & display. In ticket master installation date is 20/10/2019, As per stock book the equipment is installed on 30-08-2019 Aged up to 4 Years and 7 months. Quotation not submitted since spares not available in market. So we recommending the equipment for condemnation
17	Name & Signature of CYRIX Authority	GOKUL KT 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Verified with the damage of board & display. Beyond economic repair.





31/7/24

Signature of JC BM (NHM)
Jr. Consultant Biomedical Engineer



Date: 6/7/2024


Medical Officer
Superintendent
F.H.C. Nannambra
P.O. Kodinhi - 676 309
Medical Officer (i/c)



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 184478

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>PHC</u></p> <p>Address <u>NANNAMBRA</u> <u>MALAPPURAM</u></p> <p>Ph : <u>9207112247</u></p>	<p>Call Registration Date : <u>5/06/2024</u></p> <p>Caller ID : <u>115320</u></p> <p>Date of Visit : <u>6/6/24</u></p> <p>Asset No. : <u>1041231</u></p> <p>EQPT Name : <u>weighing machine</u></p> <p>Manufacture <u>Scms 0</u> Model : <u>NA</u></p> <p>S. No. <u>NA</u> Dept. <u>OP</u></p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : weighing machine not working.

Action Taken : Checked the machine and found problem board and display. need to replace these spare for further checking.

Completed Date : 6/6/24 Time : 12:00pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>CORUL K-T</u>	<u>6/6/24</u>	<u>11:15am</u>	<u>12:00pm</u>





Customer Remark Completed Pending


Engineer Name : CORUL K-T
Signature : [Signature]
Date : 6/6/24
Contact Number : 9809314280

Customer Name : Araghane.kp
Signature : [Signature]
Date : 6/6/24
Contact Number : 9207112247
Designation : N/O
Hospital Seal :



Office
Nannambra
9809314280

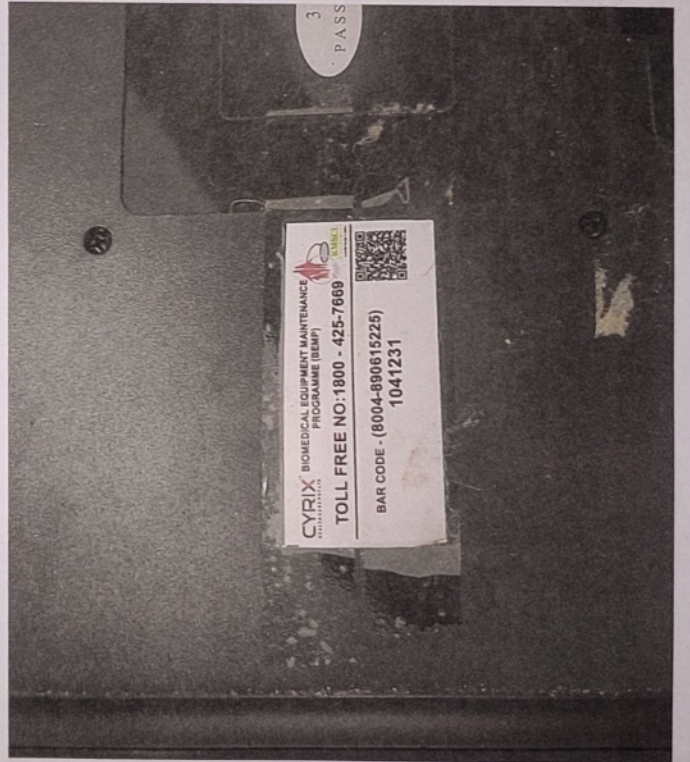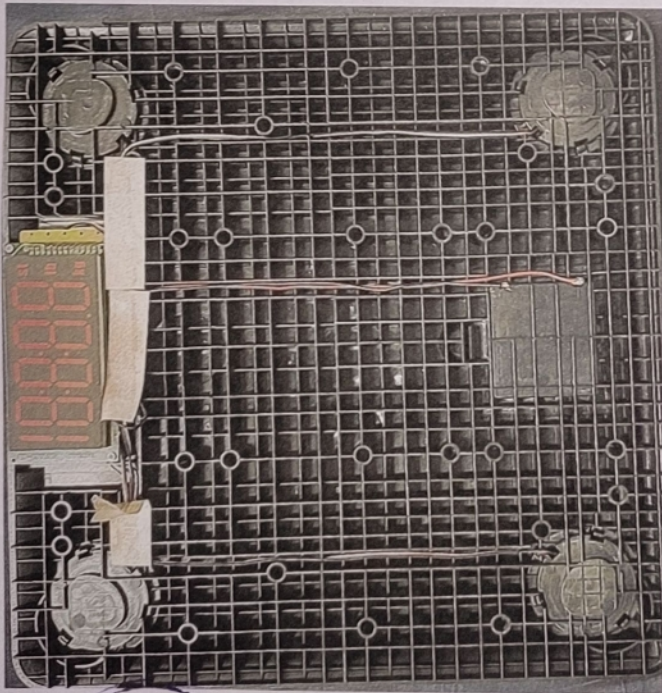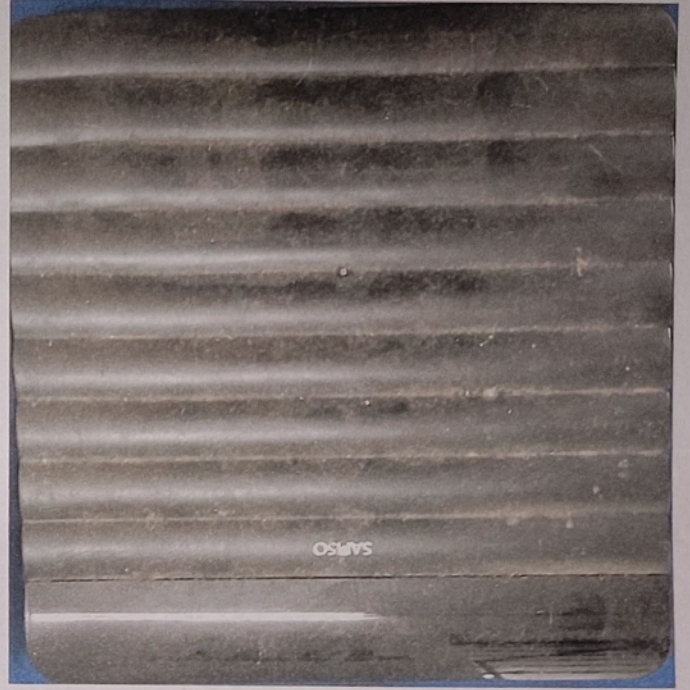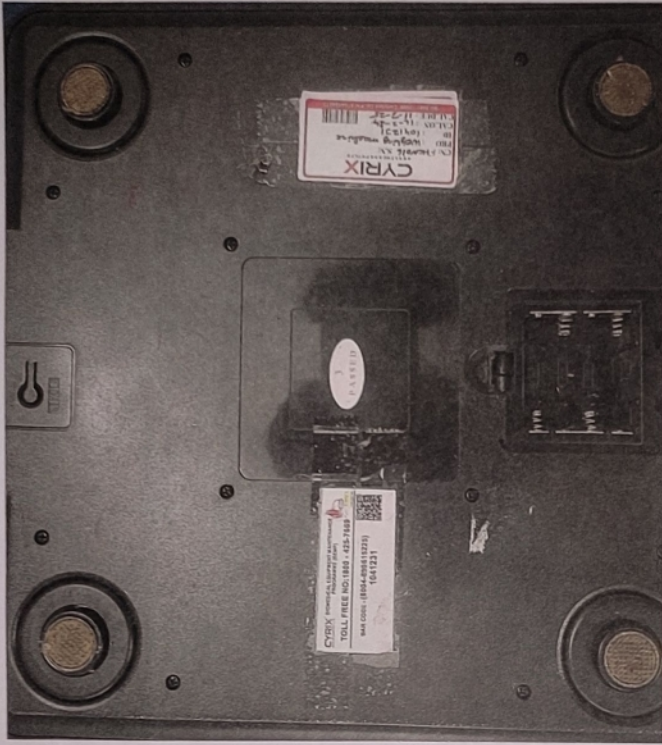


 Medical Officer
 F.H.C Nannambra
 P.O. Kodinhi - 676 309