


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

<b>Sl. No</b>	<b>Particulars</b>	<b>Details</b>
1	Name of District	Wayanad
2	Name of Hospital	PHC Appappara
3	Name of Equipment with Make, Model and Serial Number	Equipment- UPS Make-APC by Schneider electric Model- BX 600C-IN Sn-F21640002093
4	Equipment ID/ Barcode	1240127//TICKET 119109
5	Date of purchase/ Year of manufacture/Installation Date	01/09/2017
6	Warranty details (Yes/No)	NO warranty
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	25/06/2024-TOLL FREE
9	Action taken	Checked and found Main board and battery defective, Need to replace these spare for further checking. Enquired to supplier for quotation
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendation
12	Cost of spares (specify parts and cost)	600VA/12V Board replacement-3000/- 7Ah battery-1500/- <b>Total-4500/-</b>


13	Asset Value	4500/-
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	100%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Quotation from local vendor (Hybrid solar kalpetta) Cyrix service report
16	Reasons for recommending the equipment as BER	Checked the equipment and found main board and battery defective. Equipment installed on 01/09/2017 aged up to 6 years 9 months. Repairing cost is 100% both criteria for RBER met. As per tender clause 5.3.14.1 we recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	NIYAS HADI AP 


\*Not mandatory #Based on the period of life and value as per the BER guidelines


\* **Attach Photograph**

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Main board and battery are damaged. Medical  
Cost exceeds around 100%. Recommended  
replacement.

  
CONSULTANT  
Signature of Junior Biomedical Engineer  
National Health Mission  
(Arogyakeralam)  
Wayanad-673122

  
Signature of Superintendent Medical Officer (M.O.)  
കുടുംബാരോഗ്യ കേന്ദ്രം, വയനാട് - 670 645

  
FAMILY HEALTH CENTRE  
APPAPARA, WAYANAD - 670 645  
Date: 18/11/2017



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

No. : 220860

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.ki@cyrix.in

<p>Health Facility ..... <u>PHC</u> .....</p> <p>Address ..... <u>APPAPPARA</u> .....</p> <p>..... <u>WAYNAD, KERALA</u> .....</p> <p>Ph : ..... <u>9946981398</u> .....</p>	<p>Call Registration Date : ..... <u>25/6/2024</u> .....</p> <p>Caller ID : ..... <u>119189</u> .....</p> <p>Date of Visit : ..... <u>2/7/2024</u> .....</p> <p>Asset No. : ..... <u>1240127</u> .....</p> <p>EQPT Name : ..... <u>UPL</u> .....</p> <p>Manufacture ..... <u>APC</u> ..... Model : <u>BX-600C</u> .....</p> <p>S. No. <u>F216400.2</u> Dept. <u>LAB</u> .....</p>
--	---

**Service Classification :** Breakdown Call  PMS  Calibration  Cust. Training

**Problem Identified :** Not switching on

**Action Taken :** Inspected the equipment. Found that main board and battery faulty. Need to replace the both.

Completed  Date : ..... Time : ..... Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1. MAIN BOARD	1		
2. BATTERY	1		
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Dijulim</u>	<u>2/7/2024</u>	<u>1:30PM</u>	<u>2:30PM</u>

**Customer Remark** Completed  Pending



**Service Engineer Name** Dijulim

Signature: [Signature]

Date: 2/7/2024

Contact Number: 8826753545

**Customer Name** [Signature]

Signature: [Signature]

Date: 2/7/2024

Contact Number: 9946981398

Designation: LT

Hospital Seal: [Seal]

**HYBRID  
SOLAR**

Near KFWW Board, Kalpetta Wayanad  
Mob: 8089386389, 9745772211

HS/189/23-24  
11/08/2024

TO  
THE CYRIX HEALTH CARE  
KOCHI

Attn: Sir,  
Ref :


SUB: -


Ref: - As Per Your Enquiry Notice No:

We are pleased to quote our UPS & Battery Service Price as below

SLNo	Description	Rate	Qty	Amount
1	600VA/12V BOARD REPLACEMENT	3000.00	1	3000.00
2	7AH BATTERY REPLACEMENT	1500.00	1	1500.00
	INCLUDING SERVICE CHARGE			
<b>TOTAL</b>				<b>4500.00</b>

Yours truly  
For Hybrid Solar  
Kalpetta  
Wayanad  
E-mail: hybridsolar8911@gmail.com



For Mr  
  
രബീക്കുൾ ഹൈന്ദവ  
കുടുംബ ആരോഗ്യ കേന്ദ്രം  
അപ്പപ്പാ, വയനാട് - 670 646



**500Va ups complaint at phc Appappara, Wayanad(barcode-1240127)**

2 messages

**Niyas Hadi AP** <niyascyrix@gmail.com>  
To: hybridsolar8911@gmail.com  
Cc: DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>

Thu, 11 Jul 2024 at 9:31 am

Dear Sir  
A 600 VA online ups complaint reported at phc Appappara, wayanad  
Please attend the complaint and revert back with service quotation at the earliest  
Equipment -600VA ups  
Make -APC  
model -UPS600

Thanks & regards

NIYAS HADI  
District incharge  
BEMP project  
Wayanad  
kerala  
mob -7593847171

email -niyascyrix@gmail.com

www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd

| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India

KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

**Anoop PK** <hybridsolar8911@gmail.com>  
To: Niyas Hadi AP <niyascyrix@gmail.com>  
Cc: DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>


Mon, 15 Jul 2024 at 12:02 pm

Dear Sir  
Our technician attended the complaint and found main board faulty and battery defective  
Please find attached quote for the service  
[Quoted text hidden]

*For mo*  
*[Signature]*

മെഡിക്കൽ ഓഫീസർ  
കുടുംബ ആരോഗ്യ കേന്ദ്രം  
അപ്പപ്പാറ, വയനാട് - 670 646



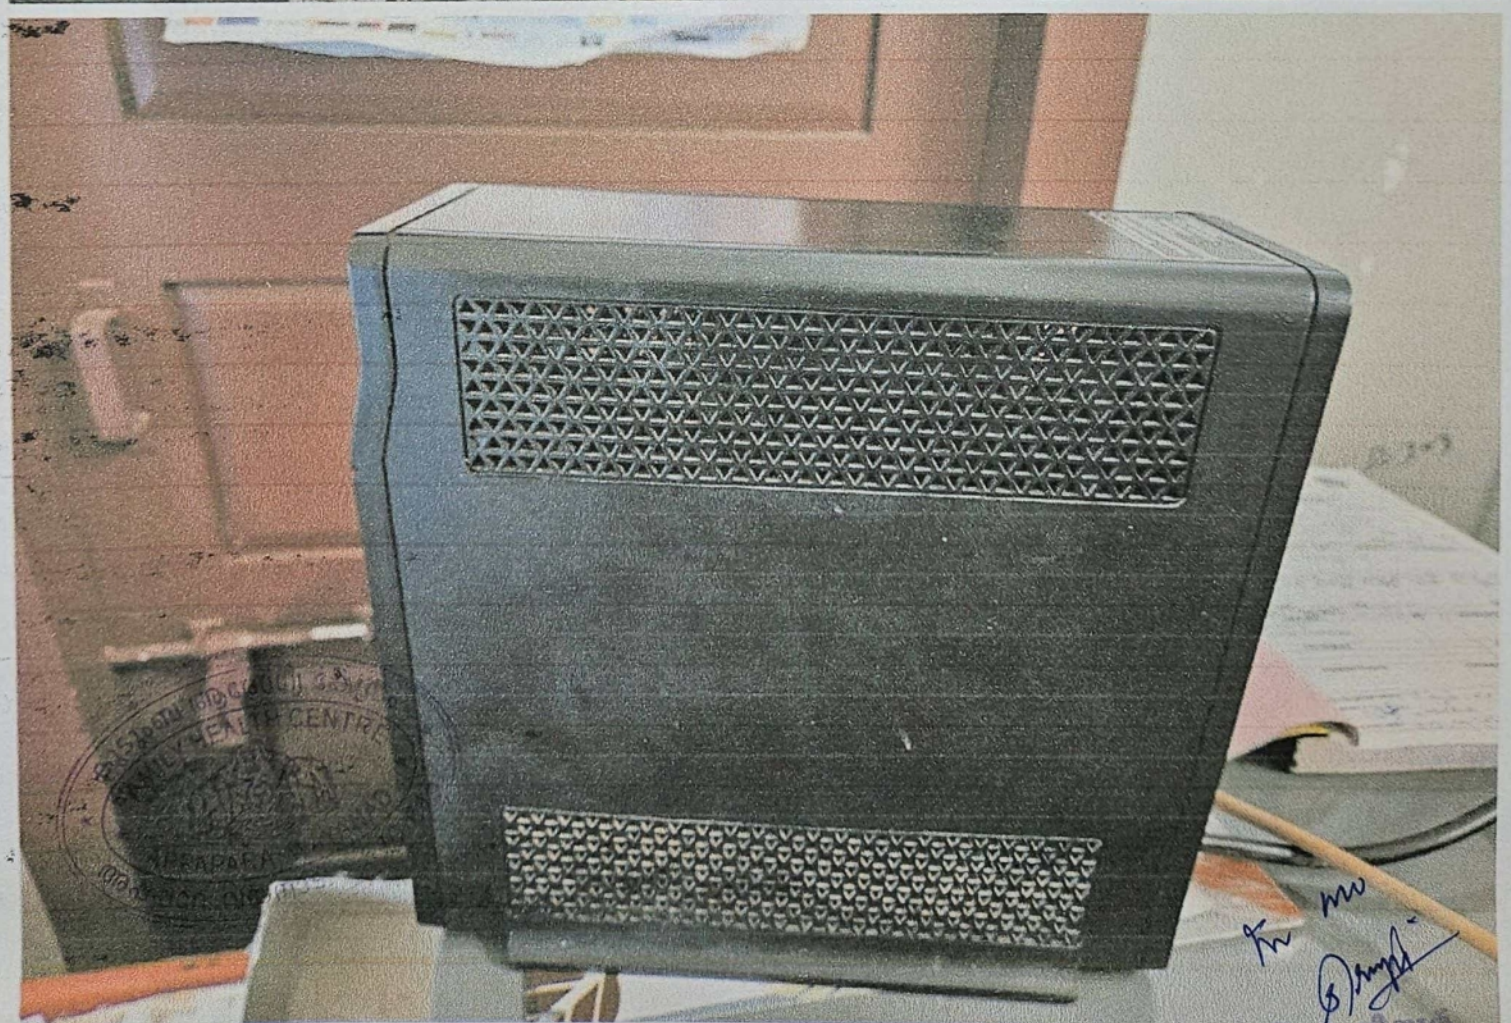

*K. M. S. Prasad*  
 മെഡിക്കൽ സെമിനാർ  
 കൃഷ്ണ ആരോഗ്യ കേന്ദ്രം  
 അപ്പപ്പാറ, വയനാട് - 670 623

ROBONIK PRIETEST TOUCH - 1  
with UPS

Seen ✓

UPS - not working - Sent to Karpatti

21/8/17  
BIF Form p.no. 256  
of sub stock register  
p.p. 1

By Condensation. on 25/11/18  
ROBONIK BARCODE : 67120851

1/9/17 MISRA VIVA  
(AGADRE)  
with UPS

INSTALLATION DATE 01/11/2017.

INVOICE TOTAL → 59,787/-

SERIAL NO : 2.1173021872.

INVOICE NO : CO-1718-SINV-001675

" DT : 08/08/2017

BIF form p.no. 56 of sub stock register  
Vol I. Balance - 1 No.



Handwritten signature and initials.

മെഡിക്കൽ ഓഫീസർ  
കുടുംബ ആരോഗ്യ കേന്ദ്രം  
അപ്പാര, നയനാട് - 670 646