



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

# CYRIX

HEALTHCARE PVT LTD

**No. :** 218145

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>General Hospital</u></p> <p>Address <u>Thiruvananthapuram</u> <u>Kerala</u></p> <p>Ph : <u>9746673761</u></p>	<p>Call Registration Date : <u>13/5/2024</u></p> <p>Caller ID : <u>110788</u></p> <p>Date of Visit : <u>13/5/2024</u></p> <p>Asset No. : <u>0150483</u></p> <p>EQPT Name : <u>BP Apparatus</u></p> <p>Manufacture <u>Elko meter</u> Model : <u>NI1</u></p> <p>S. No. <u>412648</u> Dept. <u>Casualty</u></p>
---	--

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** BP apparatus not working - mercury leak

**Action Taken :** checked and found that hinges got broken inside the holder, Mercury leak and glass rod found damage. Need to replace these spars for further checking.

Completed  Date : 13/5/24 Time : 3:35 PM Spare Required

Spare Replaced  Requested

No.	Description	Qty.	Part Number	PR Number
1.	NA	NA	NA	NA
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Sooya Sudheep</u>	<u>13/5/24</u>	<u>3:30 PM</u>	<u>3:50 PM</u>

Customer Remark  Completed



<p>Service Engineer Name : <u>Sooya Sudheep</u></p> <p>Signature : <u>Sooya</u></p> <p>Date : <u>13/5/24</u></p> <p>Contact Number : <u>7907406244</u></p>	<p>Customer Name : <u>Vijeth Vijayan</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>[Date]</u></p> <p>Contact Number : <u>9188006735</u></p> <p>Designation : <u>N/A</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
--	---

Sub-intendent  
General Hospital  
Thiruvananthapuram

REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)


Recommendations for Beyond Economic Repair (BER)

512

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	GENERAL HOSPITAL THIRUVANANTHAPURAM
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : BP Apparatus Manufacturer : Anita Industries Model:Elkometer Sl: 412648
4	Equipment ID/ Barcode	110788/ 0150483
5	Date of purchase/ Year of manufacture/Installation Date	28/06/2017
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	13/05/2024 (Toll free)
9	Action taken	Checked the found mercury spillage, identified glass rod defective and hinges screw broken inside the socket.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not recommending for Repair
12	Cost of spares (specify parts and cost)	Not available



13	Asset Value	Rs . 1323/-
14	Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	Na
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment RBER	Checked and found mercury spillage. Identified glass rod defective and hinges screw broken and stuck inside the holder screw socket. The apparatus is installed on 28/06/2017 and covered upto 6+ years. Quotation not attached since the mercury is not available in the market, recommending for condemnation.
17	Name & Signature of CYRIX Authority	Kasyep PV 

\*Not mandatory #Based on the period of life and value as per the BER guidelines

\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

*glass rod broken . So can be RBER.*

**MANEESHA MOHAN M.R.**  
Junior Consultant (Biomedical)  
National Health Mission  
Thiruvananthapuram

*MB*  
12-06-2024

Signature of JC BM (NHM)

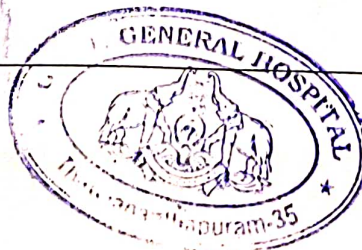


Date:

Signature of  
Superintendent/Medical Officer (i/c)

Superintendent  
General Hospital  
Thiruvananthapuram




# SPHYGMO MANOMETER.

		B	R	B	Page
9.6.13	BF ofel Reg vol. 2 Page No 187, 208, 125, 207,			21	
	Condemned As Per order No CP /10794/2012/GIT DTD 18/2/13 No-3.			18	
27.8.13	Issued from Stone RS-1748/		2	20	
7-12-13	Received from Stone Vol 8 AB - P. 83 RS - 1714/-30. Ps		1		
23.1.14	Received from Stone Vol 8 AB - P 83 RS - 1714/30 Ps		1	22	
24-1-14	BP apparatus transferred to RMO'S Room (Condemned - 11)			21	
12.5.14	Received from Stone - Vol 8 A Page 143 -		2	23	
	Condemned and disposed as per order no CH 5229/2014/GIT dated 3/8/2015 11 nos			12	
12/4/16	Received from Stone Vol 8 A page 144 condemned & disposed as per order no CH 7421/Phase 4 dated 19/12/18 (10 nos)		3	15	
16/3/17	Received from Stone IR Vol: 80 page No: 62			7	62
22/6/17	Recd from Stone Page No: 301 Vol: IR & R			9	
12/17	Received from Stone (Amal) SPRA 302				

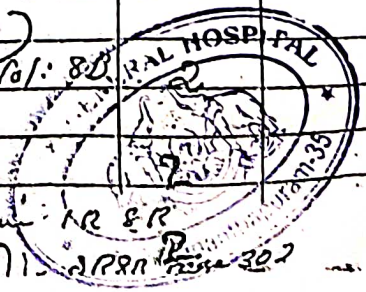

Srinivasan Hospital  
Srinivasan Hospital  
Srinivasan Hospital



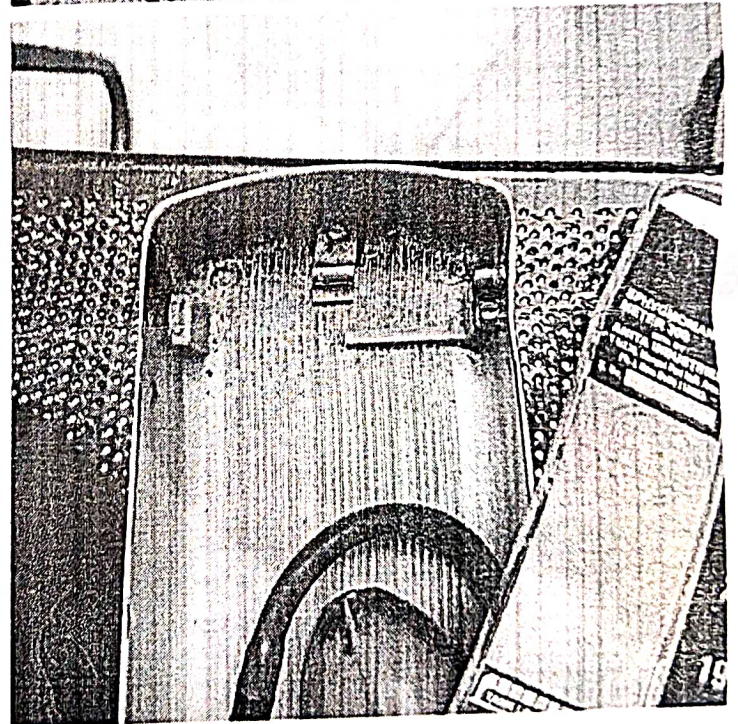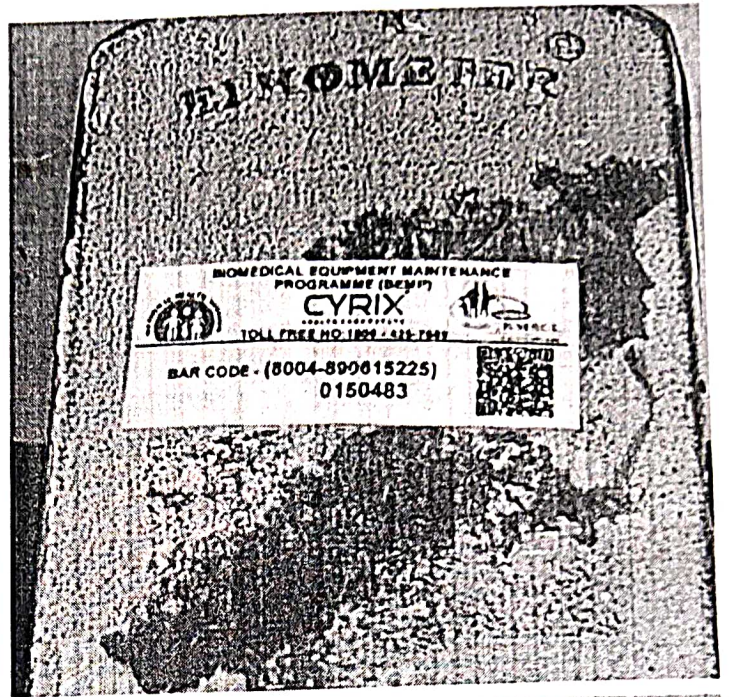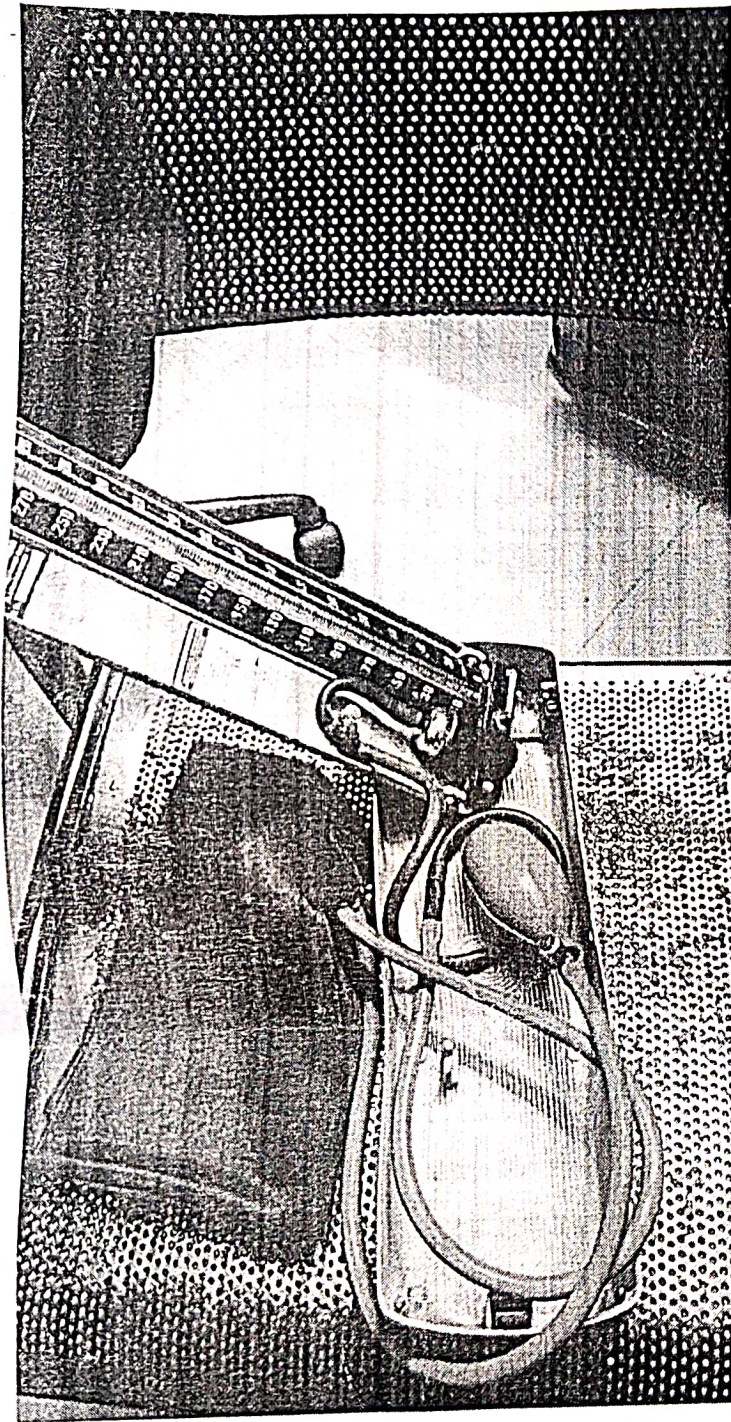

*[Handwritten Signature]*  
Superintendent  
General Hospital  
Thiruvananthapuram