



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 205700

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>THCOH</u></p> <p>Address <u>Attungal</u> <u>Thiruvananthapuram</u></p> <p>Ph : <u>8075496606</u></p>	<p>Call Registration Date : <u>21/05/2024</u></p> <p>Caller ID : <u>112235</u></p> <p>Date of Visit : <u>18/06/2024</u></p> <p>Asset No. : <u>0120158</u></p> <p>EQPT Name : <u>BP Apparatus</u></p> <p>Manufacture <u>Omron</u> Model : <u>NA</u></p> <p>S. No. <u>NA</u> Dept. <u>Labour Room</u></p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : NOT WORKING - BP Reading issue

Action Taken : Checked and Found mainboard and pump defective. Need to Replace these spare for further checking and working condition of the unit

Completed Date : 18/06/24 Time : 10:00am Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Deepak. E.M</u>	<u>18/6/24</u>	<u>10.30</u>	<u>11am</u>

Customer Remark Completed Pending

<p>Service Engineer Name : <u>Deepak</u></p> <p>Signature : <u>Deepak</u></p> <p>Date : <u>18/06/24</u></p> <p>Contact Number : <u>7902881038</u></p>	<p>Customer Name : <u>N Debu BS</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>18/06/24</u></p> <p>Contact Number : <u>703485000</u></p> <p>Designation : <u>Staff Nurse.</u></p> <p>Hospital Seal : </p>
---	---

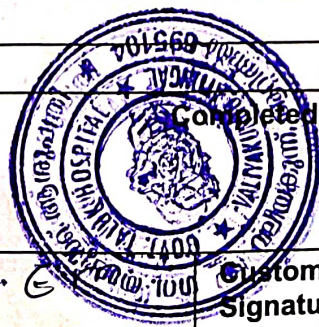

Superintendent
Taluk Hospital
Attungal

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

521

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	THQH ATTINGAL
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : BP Apparatus Make : Omron Model : HEM-7120 Serial No : NA
4	Equipment ID/ Barcode	0120158/112235
5	Date of purchase/ Year of manufacture/Installation Date	08/03/2018
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	21/05/2024
9	Action taken	Checked and found mainboard and pump defective. Need to replace these spares for further checking and working condition of the unit.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE

13	Asset Value	2200/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	Not Available
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found Mainboard and pump defective. The apparatus is installed on 8/3/2024 and covered upto 6+ years. Since the spares are not available in the market. As per the tender clause 5.3.14.2, recommending the unit for condemnation
17	Name & Signature of CYRIX Authority	KASYEP PV

*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Main board and pump defective. So as per tender conditions; recommended beyond economic repair

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram

JPB
22-06-2024

Signature of JC BM (NHM)

Date: _____



Signature of
 Superintendent/Medical Officer (BM)
 Government Medical Hospital
 Thiruvananthapuram
[Handwritten Signature]

Digital B.P. Apparatus

233

Rld

Serial Number




		Rld	Serial	Number
28/7/18 8/3/2018	Recd from stock Digital		1	1
10/2/2020	Received from Stock (main stock page no. 392 volume 6)	1		2 copy
27/6/2022	Received from stock (Donation Register Page no: 39 Vol. I)	1		3 copy
2/3/24	Rld from store kept in use	1	1	4 copy

Jagadeesh
18/04/24
PHARMACIST & STORE KEEPER
TALUK HOSPITAL ATTINGAL



[Handwritten signature]

Superintendent
Taluk Hospital
Attingal

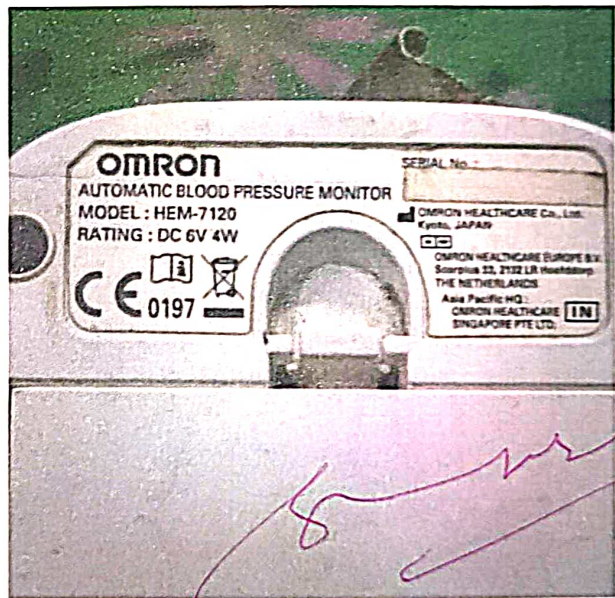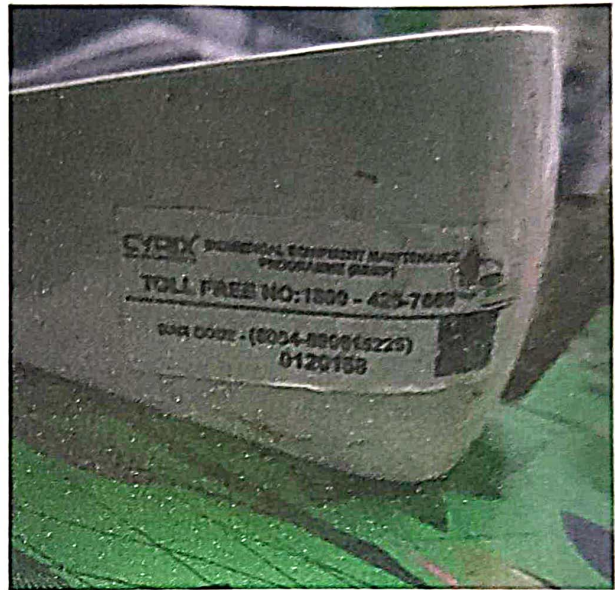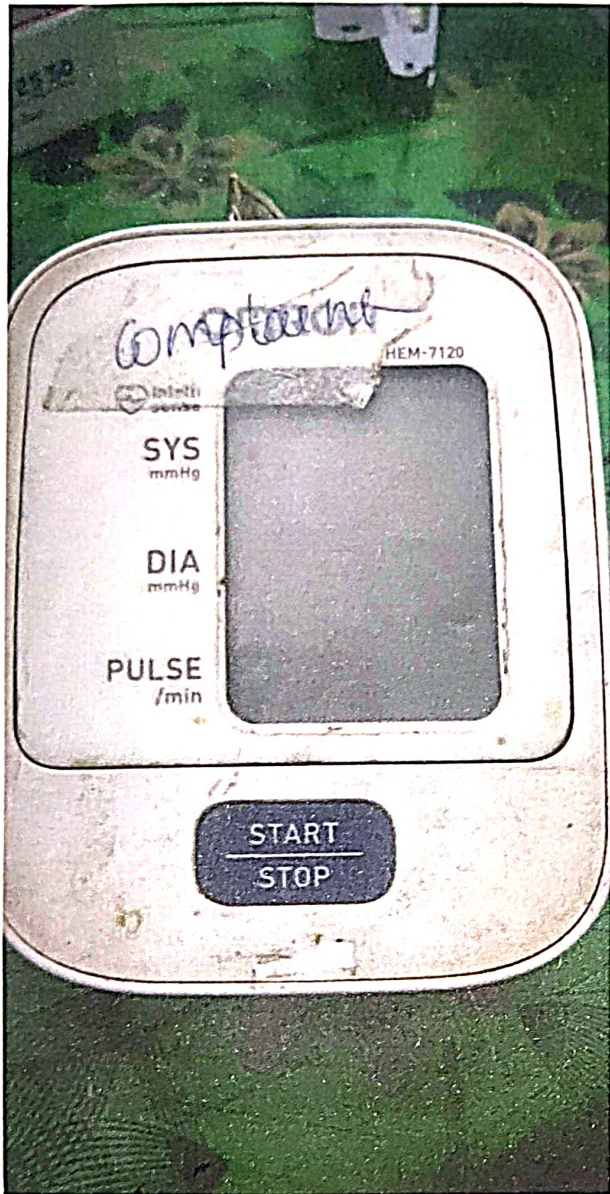

8/16/6-



**Superintendent
Taluk Hospital
Aringai**