


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KOZHIKODE
2	Name of Hospital	PHC ARIKKULAM
3	Name of Equipment with Make, Model and Serial Number	Equipment : NEBULIZER Make: LIFE CARE Model: CNB69022 SN : NA
4	Equipment ID & Barcode	121587 & 1142366
5	Date of purchase / Year of manufacture /Installation Date	installation date is 13-09-2019
6	Warranty details (Yes/No)	NO Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	06-07-2024
9	Action taken	Checked and found compressor motor with piston defective. Need to replace these spares for further checking of working condition of the equipment
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	1875/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found compressor motor with piston defective. Need to replace these spares for further checking of working condition of the equipment Machine installed on 13-09-2019 aged up to 04 years 10 month. Quotation not submitted since spares are not available in the market So we recommend the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AKHILRAJ MP 

*Not mandatory

#Based on the period of life and value as per the BER guidelines


* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Checked & found that motor with piston defective. Machine is installed on 13/9/2019. Spares are not available in the market. So recommended for condemnation

Signature of JC BM (NHM)
 Consultant Bio Medical
 National Health Mission
 Kezhikode

Date



Signature of **Medical Officer**
Family Health Centre
 Superintendent / Medical Officer



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 144007

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>PHC Arikkulam</u>.....</p> <p>Address <u>Arikkulam</u>..... <u>Kozhikode</u>.....</p> <p>Ph : <u>9539751747</u>.....</p>	<p>Call Registration Date : <u>6/7/24</u>.....</p> <p>Caller ID : <u>121587</u>.....</p> <p>Date of Visit : <u>8/7/24</u>.....</p> <p>Asset No. : <u>1142366</u>.....</p> <p>EQPT Name : <u>nebulizer</u>.....</p> <p>Manufacture <u>Life care</u>... Model : <u>CNB.69022</u></p> <p>S. No. <u>LC22190401747</u> Dept. <u>OP</u>.....</p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified :

fumes not getting

Action Taken : checked & found that compressor motor with piston defective, need to replace these spares for further checking the working condition of this equipment.


Completed Date : 8/7/24 Time : 5:05pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. _____			
2. _____			
3. _____			


Cyrix Engineer	Date	Start Time	End Time
<u>Akhilraj</u>	<u>8/7/24</u>	<u>4:30pm</u>	<u>5:05pm</u>

Customer Remark Completed Pending



Service Engineer Name : Akhilraj
[Signature]
Date : 8/7/24
Contact Number : 9843677676

Customer Name : Reshma ghy
Signature : [Signature]
Date : 8/7/24
Contact Number : 9843677676
Designation : Medical Officer
Hospital Seal : Family Health Centre Arrikulam

Compressor Nebulizer  Lifecare™
 Model No.: CNB69022
 Input : AC-220V/50HZ
 Power : 180VA
 Serial No.:
 Mode of operation-continuous
 No AP/PG IPXO




BIOME	10-650	907579)-
MAINT		
(BMMI)		

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO:1800 - 425-7669
 BAR CODE - (8004-890615225) 1142366



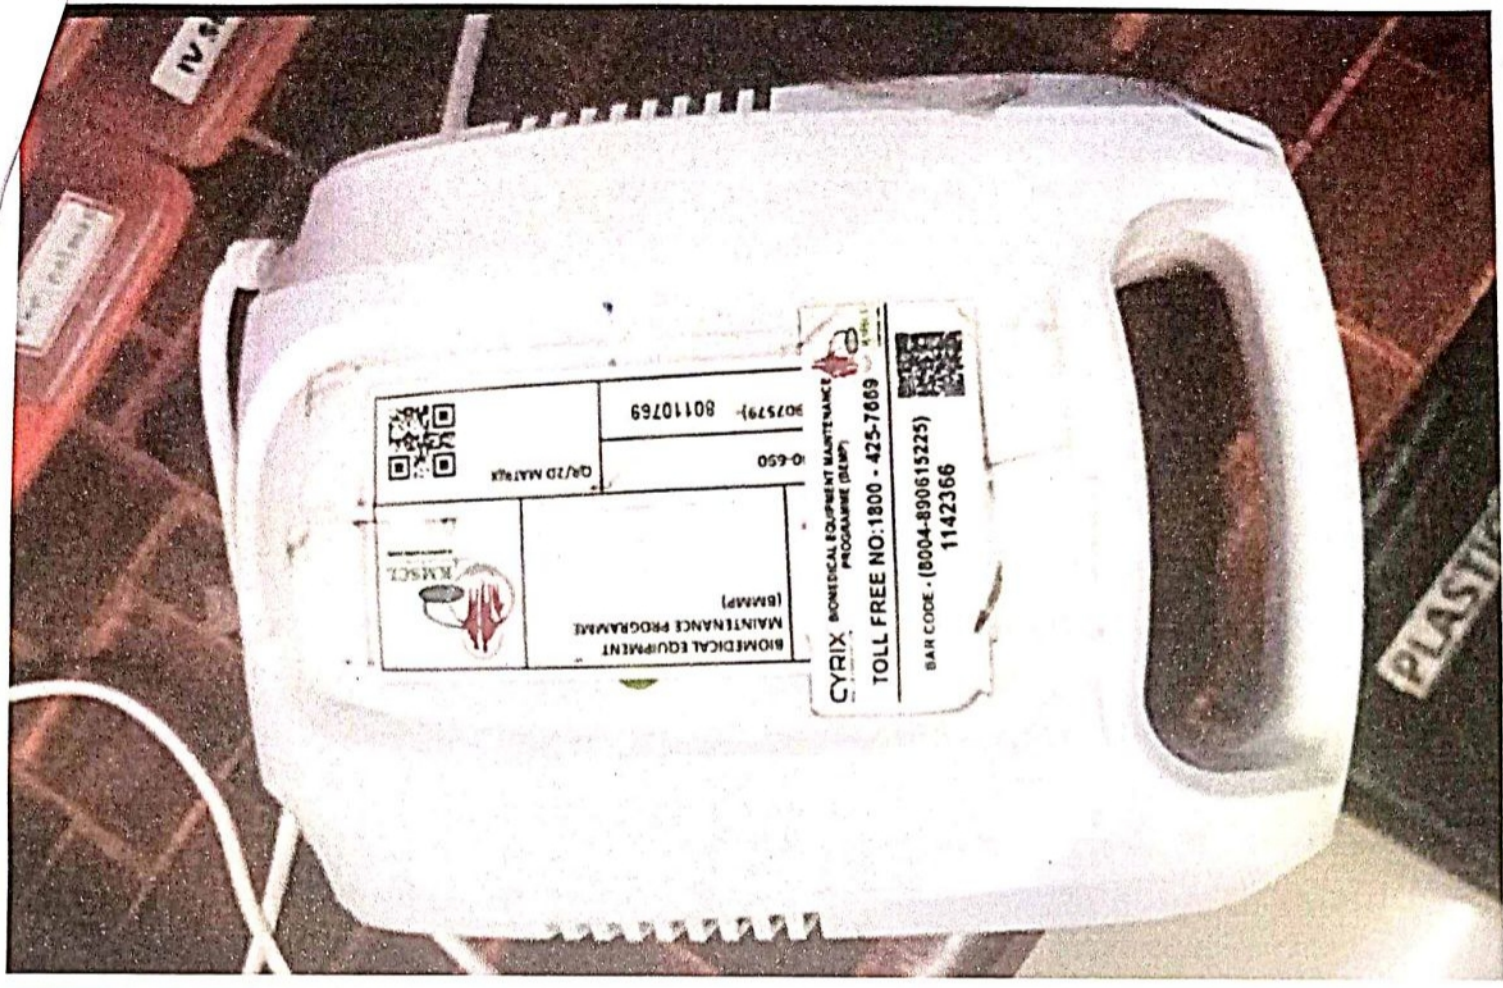

Medical Officer
 Family Health Centre
 Arikkulam



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)	10-650	907579)-
(BMMI)		
MAINTENANCE PROGRAMME		
BIOMEDICAL EQUIPMENT		

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
TOLL FREE NO:1800 - 425-7669
 BAR CODE - (8004-890615225) 1142366



Nebulizer.

13 ⁴ / ₁₈	From KMSLW. Invoice no. 9126, dated 15 ³ / ₁₈	1		1	
15 ⁴ / ₁₈	issued to SN Deja	1		NIL	2/6/19. R BR. instruments and Furniture 6
10/9/19	From KMSLW				
10/9/19	From KMSLW Medicine depot. Pluva - Invoice NO 6047, Date 10/10/19 with waracolicard.	1		1	Exp dt Jan 2025 Rate - 12321 MRP - 3100 Batch 113
12/9/19	Issued to SN Deja & with waracolicard.			1	NIL
10/9/19	From KMSLW Medicine depot Pluva - Invoice NO - 8506 Date 26/8/2019	1		1	Exp dt - Jan 25 Batch 113 Rate - 12321 MRP - 3100
13/9/19	Issued to SN Deja with waracolicard			1	NIL

MEDICAL OFFICER
FAMILY HEALTH CENTRE, ARIKKULAM
KERALA HEALTH SERVICE
KOZHIKODE, KERALA

[Handwritten Signature]

**Medical Officer
Family Health Centre
Arikkulam**

