


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

<b>Sl. No</b>	<b>Particulars</b>	<b>Details</b>
1	Name of District	KANNUR
2	Name of Hospital	CHC KARIVELLUR
3	Name of Equipment with Make, Model and Serial Number	SEMI AUTO BIOCHEMISTRY ANALYZER Make: ROBONIK Model: PRIETEST TOUCH SN: AT1100111RBK
4	Equipment ID/ Barcode	1330033 #117877
5	Date of purchase/ Year of manufacture/Installation Date	Ticket master installation date - 16-03-2011 ( As per stock book installation date is 07.06.2011)
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free 19-06-2024
9	Action taken	Checked the machine and found that Machine is not switching ON, found problem with primary board, enquired OEM for quotation
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	N/A

13	Asset Value	64760/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report & OEM End of life letter attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that Machine is not switching ON, found problem with primary board, enquired OEM for quotation. In ticket master installation date is 16-03-2011 and As per stock book installation date is 07.06.2011 equipment aged up to 14 years. OEM informed that this machine is obsolete model, end of life letter issued. As per tender clause 5.3.14.2 we recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AVINASH T 

\*Not mandatory #Based on the period of life and value as per the BER guidelines

\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Checked the machine & found that not switching ON, as per OEM letter it is an obsolete model. Also aged up to 14 years. So recommended for BER as per BER protocol.

  
04/07/2024 Signature of JC BM (NHM)




Nimisha. k.P



17/7/2024

Nursing officer Gr.I

Date: 17/7/24

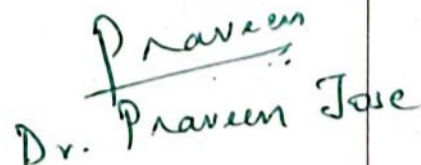  
Dr. Praveen Jose

MEDICAL OFFICER  
Sig. COMMUNITY HEALTH CENTRE  
Superintendent KARNVELLUR-670521



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

# CYRIX

HEALTHCARE PVT LTD

**No. :**  
227470

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility ..... <u>CHC Karivellur</u> .....</p> <p>Address ..... <u>Kannur</u> .....</p> <p style="padding-left: 40px;"><u>Kerala</u> .....</p> <p>Ph : ..... <u>9526484240</u> .....</p>	<p>Call Registration Date : <u>19-06-2024</u> .....</p> <p>Caller ID : <u>117877</u> .....</p> <p>Date of Visit : <u>20-06-2024</u> .....</p> <p>Asset No. : <u>1330033</u> .....</p> <p>EQPT Name : <u>Biochemistry Analyzer</u> .....</p> <p>Manufacture <u>Robonik</u> Model : <u>Poietest Touch</u></p> <p>S. No. <u>AT110011RBK</u> Dept. <u>Laboratory</u> .....</p>
--	--

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** found machine is not switching ON.

**Action Taken :** Checked the machine and found that machine is not switching ON, found problem with primary board, enquired OEM for quotation.

Completed  Date : 20-06-2024 Time : 11:00AM Spare Required

Spare Replaced  Requested

No.	Description	Qty.	Part Number	PR Number
1.	<u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Nitheesh P</u>	<u>20-06-24</u>	<u>10:00AM</u>	<u>11:00AM</u>

**Customer Remark** Completed  Pending

*Praveen*  
17/7/24  
MEDICAL OFFICER  
COMMUNITY HEALTH CENTRE  
KARIVELLUR-670 521

<p><b>Service Engineer Name :</b> <u>Nitheesh P</u></p> <p><b>Signature :</b> <u>[Signature]</u></p> <p><b>Date :</b> <u>20-06-2024</u></p> <p><b>Contact Number :</b> <u>830184153</u></p>	<p><b>Customer Name :</b> <u>[Signature]</u></p> <p><b>Signature :</b> <u>[Signature]</u></p> <p><b>Date :</b> <u>20/6/24</u></p> <p><b>Contact Number :</b> <u>9526484240</u></p> <p><b>Designation :</b> <u>Nimukha, KP</u></p> <p><b>Hospital Seal :</b> <u>N10 Gmri</u></p>
---	---



**Date : 24.06.2024**

Dear Valued Customer,


Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1100111RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1100111RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**



Authorised Signatory

24

# STOCK REGISTER



Name of Article  
वस्तु का नाम

Semi Auto analyser

Date तिथि	PARTICULARS विवरण	Bill No. बीजक नं०	Receipt प्राप्ति	Issue देय	Balance बाकी	Remarks टिप्पणी
7/6/24	Received from store		1		1	84000
7/6/24	Issue for lab			1		Tax-3360
						<u>87360</u>
						S.P.



Praveen  
12/12/24  
MEDICAL OFFICER  
COMMUNITY HEALTH CENTRE  
KARIVELLUR-670 521

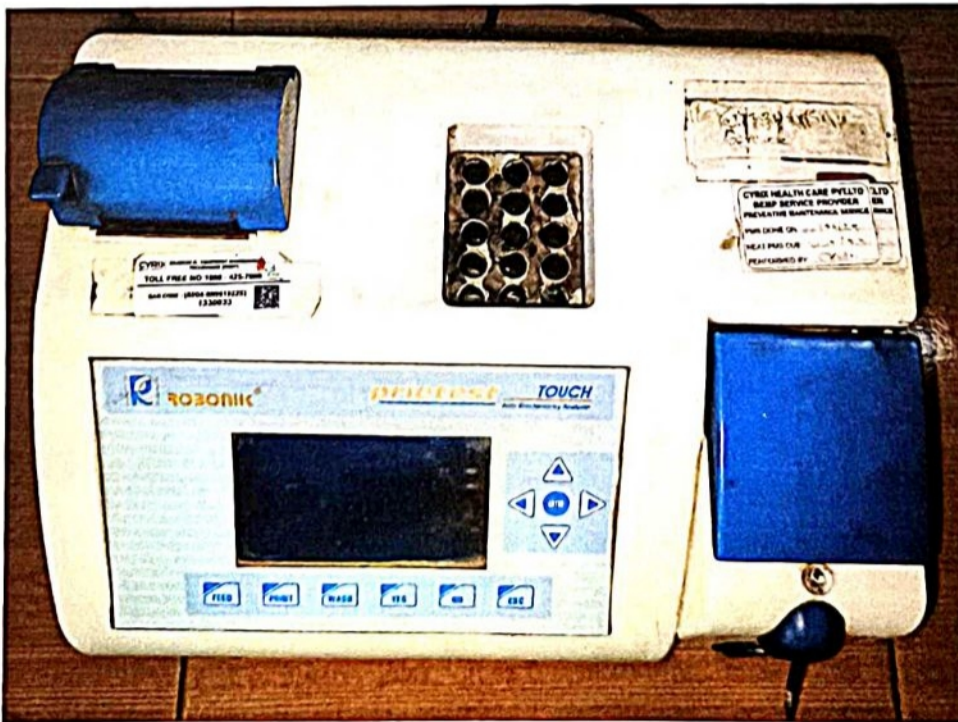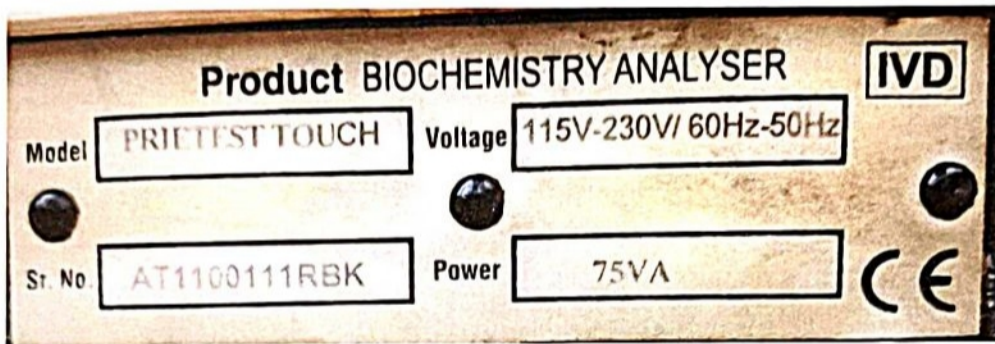

*Praveen*  
17/7/24  
MEDICAL OFFICER  
COMMUNITY HEALTH CENTRE  
KARIVELLUR-670 521