

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**


Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KANNUR
2	Name of Hospital	UDC URUVACHAL
3	Name of Equipment with Make, Model and Serial Number	UPS Make : NA Model:NA SN:NA
4	Equipment ID/ Barcode	1340217 #110504
5	Date of purchase/ Year of manufacture/Installation Date	30-06-2017
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free- 10-05-2024
9	Action taken	Checked the machine and found that Machine is already done condemnation during KTPL period.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA


MEDICAL OFFICER I/c
Urban Dialysis Centre
Uruvachal, Mattanur





13	Asset Value	2,00,000 /-
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA*
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX Service report and KTPL service report attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that Machine is already done condemnation during KTPL period on 10/11/2021, barcode-70133068, complaint no- 148837. KTPL service Report attached for reference.
17	Name & Signature of CYRIX Authority	AVINASH T 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:
 checked & identified the machine already reported as BER during KTPL time. So recommended for BER as per BER Protocol.

 25/05/2024. Signature of JC BM (NHM)
 CONSULTANT BIOMEDICAL
 NATIONAL HEALTH MISSION
 KANNUR - 670002

In BEMP quarterly review on 28/6/24 decided to physically verify the equipment by Mattannur MO. But purchase still pending. So acknowledge this remark as BER.


 15/07/2024.
 CONSULTANT BIOMEDICAL
 NATIONAL HEALTH MISSION
 KANNUR - 670002
 Date: Signature of Superintendent/Medical Officer (i/c)

MEDICAL OFFICER i/c
 Urban Dialysis Centre
 Uruvachal, Mattannur



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :
215042

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility UDC Uruvachal</p> <p>Address Kanuru</p> <p style="padding-left: 100px;">Kerala</p> <p>Ph : 9496191350</p>	<p>Call Registration Date : 10-5-24</p> <p>Caller ID : 110504</p> <p>Date of Visit : 11-5-24</p> <p>Asset No. : 1340217</p> <p>EQPT Name : UPS</p> <p>Manufacture NA Model : NA</p> <p>S. No. NA Dept. Dialysis unit</p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Machine is already done condemnation

Action Taken : checked the machine and found that machine is already done condemnation during K.T.P.L period

Completed Date : 11-5-24 .. Time : 12:15pm .. Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Syanakrishnan	11-5-24	11:45 AM	12:15 PM

Customer Remark Completed Pending

Service Engineer Name : Syanakrishnan
Signature :
Date : 11-5-24
Contact Number : 8281188514

Customer Name : Theerthas
Signature :
Date : 11-5-24
Contact Number : 9770602657
Designation : Dialysis Technician
Hospital Seal :

MEDICAL OFFICER /
Urban Dialysis Centre
Uruvachal, Mattanur

KIRLOSKAR TECHNOLOGIES (P) LTD.

159094

SL No.:



Technology from the frontiers of medical science

SERVICE REPORT

Hospital Name & Address UPHC Borora (Usunachal UDC)	Instrument Description		Complaint details		
	Instrument Name : 20 kv Ups Gas Dielectric		Complaint No. : 148827		
	Make : Kva Tech	Date of complaint :	21/11/21	Time :	11.55
	Model : 10000000	Date of visit :	10/11/21	Time :	2.00
	Serial No. : 110940617	Date of Completion :		Time :	
Bar code : 70132065			<input checked="" type="checkbox"/> Attended	<input type="checkbox"/> Closed	

Reason for visit Break down PM Others

Problem Reported by Customer :
Nbl getting ON

Action taken by Engineer : Checked the equipment found 10kv Transformer 2 nos, IGBT (3 nos), Control board (3 nos) damaged. Repair we replace some board also damaged due to high load issue. and main control PCB and Transformer are obsolete present. In this condition the UPS is Arranged so we

Spares used: Recommended for ground connected Power. Earthing condition

Part Name	Qty.	Serial No. / Lot No.	Polarity	Volts	Remarks
			P-N		
			P-E		
			*E-N		

"Earthing voltage should not be greater than 5V. Not recommended to use any Biomedical equipment, if earthing voltage is not maintained. Get the "Earthing" rectified prior to use the equipment.

Customer Remarks, if any

Customer Name : NIRHIL K	Engineer Name : Abhilesh P
Designation : - DIAGNOSIS TECHNICIAN	Designation : Senior Engineer
Contact No. : 9492294202	Contact No. : 907060051
Date : 10/11/2021	
Signature : 	Signature :



Cochin Office: "Anugraha", Door No. 55/2652, Cheruparambath Road, Kadavembra, Cochin-682020, Kerala
 Tel: 0484-2322230
 Tollfree No.: 18862799888
 E-mail: cochin@kirtoskarmedical.com

Jalpur Office: C-306, 1st & 2nd Floor, Nirmal Nagar-C, Jyesth Ameer Road, Jalpur - 302019, Rajasthan
 Phone : 0141-4911368
 Tollfree No.: 18891624838
 E-mail: jalpur@kirtoskarmedical.com

Corporate Office: B-58, First Floor, Defence Colony, Bhasham Pknam Marg, New Delhi-110024, India
 Phone: 011-41403867, 24331368, 24331369. Fax: 011-24331367
 E-mail: delhi@kirtoskarmedical.com





Regd. Office: # 306, 3rd Floor, Money Chamber, B/23, K.H. Road, Bangalore-560027, Karnataka, India
 Phone: 080-64503855, 64503858
 Fax: 080-41318855
 E-mail: bangalore@kirtoskarmedical.com

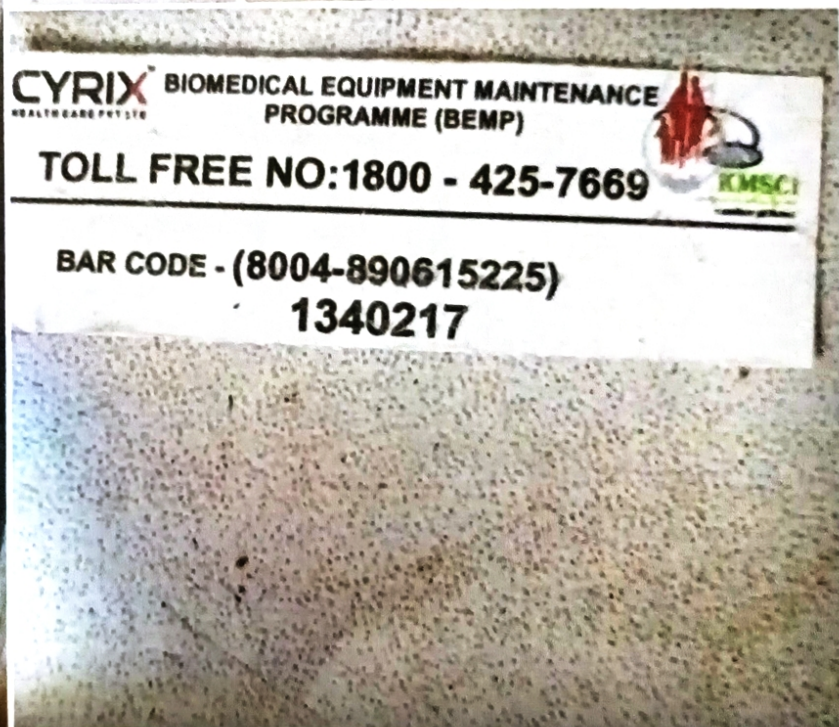
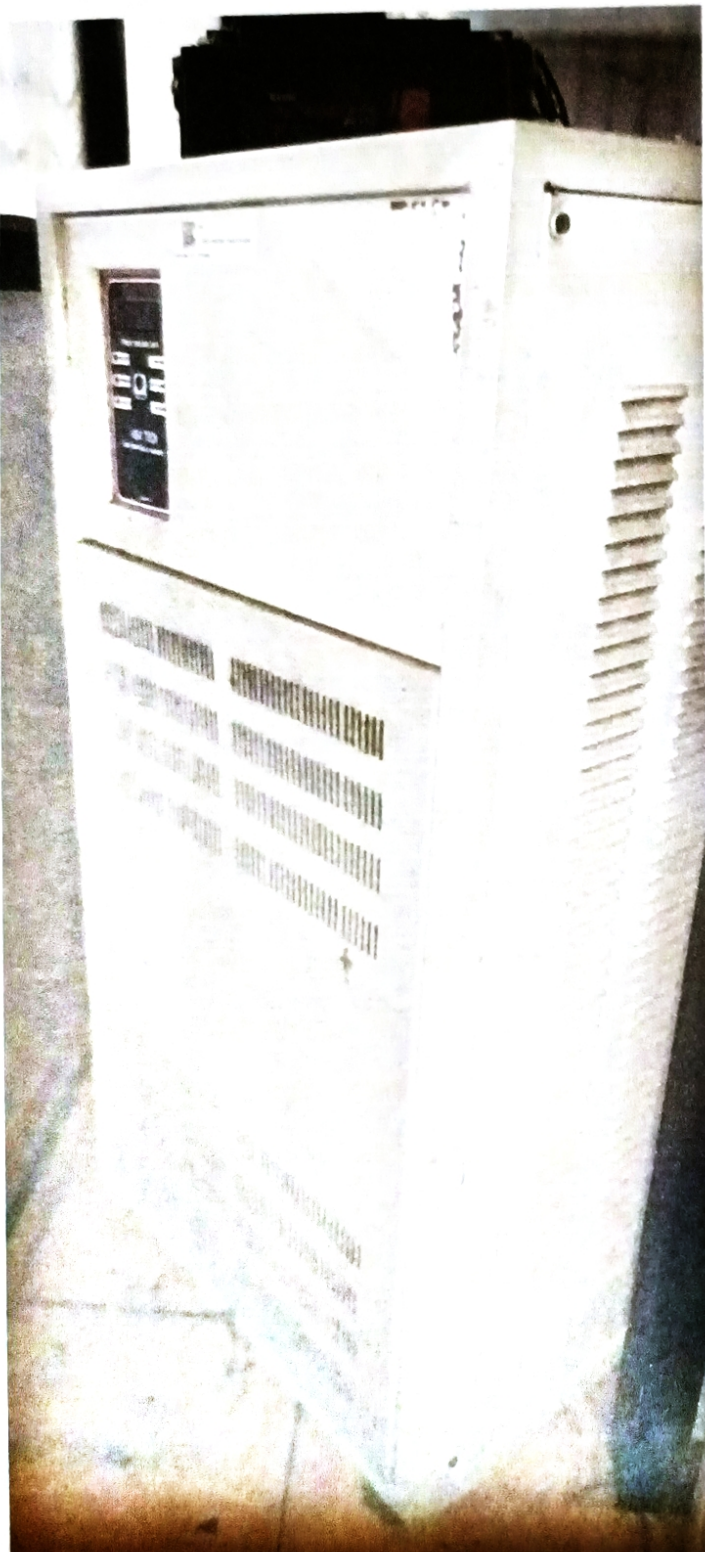
CIN : U31909KA1993PTC014893 Website: www.kirtoskarmedical.com

MATTANUR MUNICIPALITY
URBAN DIALYSIS CENTRE, URUVACHAL
STOCK BOOK OF MEDICINES AND INSTRUMENTS

55

Name of item INVERTER (HEMO UPS) 20KV

Date	From whom received or to whom issued	Receipt	Issue	Balance	Batch Number	Expiry Date	Price	Remarks
30/6/2017	<p>Received from (HLL) HLA Tech Industrial Electronics Pvt. Ltd. #11 / 230, Marathi Road, Vazhakkala Kakkannal (W) (PO), Kochi Model : 11201 20k. Serial No: M10940617</p>							
	<p>date of purchase : 30/6/2017</p>							
	<p>date of installation : 20/10/2017</p>							
	<p>One year warranty.</p>							
	<p>Barcode No: 70133068</p>							
								
								
	 <p style="text-align: right;">  MEDICAL OFFICER I/c Urban Dialysis Centre Uruvachal, Mattannur </p>							



MEDICAL OFFICER I/o
Urban Dialysis Centre
Uruvachal, Mattannur