


1010

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KANNUR
2	Name of Hospital	THQH IRITTY
3	Name of Equipment with Make, Model and Serial Number	SEMI AUTO BIOCHEMISTRY ANALYZER Make: ROBONIK Model: PRIETEST TOUCH SN: AT1070111RBK
4	Equipment ID/ Barcode	1320386 #115345
5	Date of purchase/ Year of manufacture/Installation Date	09-03-2011
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free 05-06-2024
9	Action taken	Checked the machine and found that Machine is not switching ON, found problem with primary board, enquired OEM for quotation
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	N/A

13	Asset Value	64760/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report & OEM End of life letter attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that Machine is not switching ON, found problem with primary board, enquired OEM for quotation. Equipment installed on 09-03-2011 aged up to 13 years 3 Months, OEM informed that this machine is obsolete model, end of life letter issued. As per tender clause 5.3.14.2 we recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AVINASH T 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Checked & identified that machine not switching on due to Primary board issue. Aged up to 13 years & above. OEM reported that machine is obsolete model and end of life letter. So recommended for BER as per BER protocol.


Signature of JCBM (NHM)
24/06/2024

CONSULTANT BIOMEDICAL
NATIONAL HEALTH MISSION
KANNUR - 670002

Date: 4.7.24



Signature of
Superintendent/Medical Officer (i/c)
SUPERINTENDENT
TALUK HOSPITAL IRITTY
KANNUR DT. - 670703





BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 221927

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : <u>THQH IRITTY</u></p> <p>Address : <u>Iritty</u> <u>KANNUR</u></p> <p>Ph : <u>7994 8524 74</u></p>	<p>Call Registration Date : <u>05.06.2024</u></p> <p>Caller ID : <u>115345</u></p> <p>Date of Visit : <u>06.06.2024</u></p> <p>Asset No. : <u>1320386</u></p> <p>EQPT Name : <u>SEMI AUTO BIOCHEMISTRY ANALYZER</u></p> <p>Manufacture : <u>ROBONIK</u> Model : <u>PRITEST TOUCH</u></p> <p>S. No. <u>AT107011IRBK</u> Dept. <u>LABORATORY</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Primary board is defective

Action Taken : checked the machine and found that machine is not switching ON, Found problem with primary board. enquired OEM for quotation.

Completed Date : 06.06.2024 Time : 11.30 AM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Sayanth</u>	<u>06/06/2024</u>	<u>10.00 AM</u>	<u>11.30 AM</u>

Customer Remark Completed Pending

Service Engineer Name : Sayanth
Signature : [Signature]
Date : 06/06/2024
Contact Number : 860 6 345 195

Customer Name : Soonya JK
Signature : [Signature]
Date : 06/06/24
Contact Number : 7994852474
Designation : Lab Tech. Jmdell
Hospital Seal : [Seal]



SUPERINTENDENT
TALUK HOSPITAL IRITTY
KANNUR DT. 670703



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



No. : 221927

CYRIX
HEALTHCARE PVT LTD

SERVICE PROVIDER
TANJAVUR Dt. - 612001-202198

150 15482 : 2012 & 150 15482-508 CERTIFIED COMPANY/ AERB approved Service Agency
2004 B, Puzh, Junction, Poonjar, Hoob - 605 028, Kanyakumari
PH : 98423 92800 Website : www.cyrrix.com / Email : dom@cyrix.in

Service Report

Health Facility : TALUK HOSPITAL	Call Registration Date : 08.06.2024
Address : KANNUR	Caller ID : 112345
PH : 98423 92800	Date of Visit : 08.06.2024
	Asset No. : 1320382
	EQPT Name : SEMI AUTO BIOCHEMISTRY ANALYSER
	Manufacturer : ROBENIK Model : FIRST TOUCH
	S. No. AT100111R BK Dept. LABORATORY

Service Classification: Breakdown Call PMS Calibration Cust Training

Problem Identified : Precision band is defective

Action Taken : Checked the machine and found that machine is not functioning due to found problem with precision band. Replaced band for operation.

Completed Date : 08.06.2024 Time : 11:30 AM Spare Required

Spare Replaced Requested

Description	Qty	Part Number	PR Number

Customer Remark Pending

Service Engineer Name : *[Signature]*
Signature : *[Signature]*
Date : *[Date]*
Contact Number : 98423 92800



SUPERINTENDENT
TALUK HOSPITAL
KANNUR Dt. - 612003

Date : 18.06.2024

Dear Valued Customer,

Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1070111RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT1070111RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).


Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**



Authorised Signatory

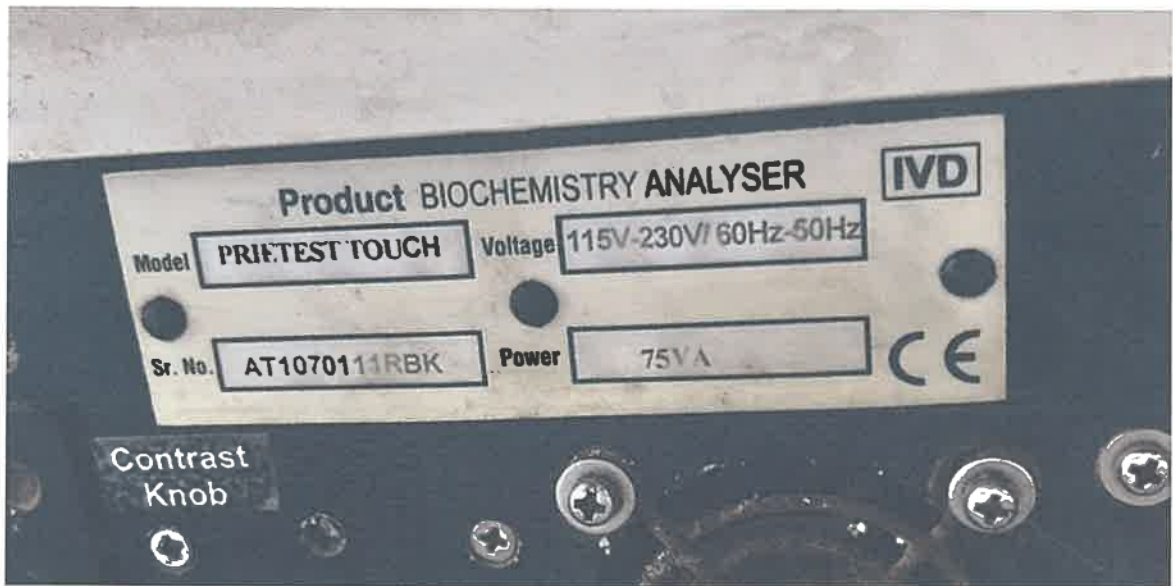

Princy
24/2/24

SUPERINTENDENT
TALUK HOSPITAL IRITTY
KANNUR DT. - 670703

