



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

No. : 223457

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERD Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 90472 98500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrrix.in

<p>Health Facility <u>UPHC Secretariate</u></p> <p>Address <u>Rajaji Nagar,</u> <u>Thiruvananthapuram</u></p> <p>Ph : <u>9895 571779</u></p>	<p>Call Registration Date : <u>5-7-2024</u></p> <p>Callor ID : <u>121407</u></p> <p>Date of Visit : <u>8-7-2024</u></p> <p>Asset No. : <u>0142953</u></p> <p>EQPT Name : <u>Nebuliser</u></p> <p>Manufacture <u>Tycheek</u> Model : <u>N8.001</u></p> <p>S. No. <u>N8.00115100</u> Dept. <u>OP</u></p>
--	--

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** Not working.

**Action Taken :** checked and found nozzle and motor side are defective. Need to replace these spares for further checking.

Completed  Date : 8-7-2024 Time : 11:30 a.m Spare Required

Spare Replaced  Requested

1.	Description	Qty.	Part Number	PR Number
2.	NA	NA	NA	NA
3.				


Cyrrix Engineer	Date	Start Time	End Time
<u>Rehna.R</u>	<u>8-7-2024</u>	<u>10:30 a.m</u>	<u>11:30 a.m</u>

**Customer Remark** Completed  Pending

**Service Engineer Name :** Rehna.R  
**Signature :** Rehna  
**Date :** 8-7-2024  
**Contact Number :** 9947239956

**Customer Name :** Dr. Reena.A.R  
**Signature :** Reena  
**Date :** 8/7/24  
**Contact Number :** 8281596348  
**Designation :** Medical Officer  
**Hospital Seal :**

NATIONAL HEALTH MISSION  
UPHC, RAJAJI NAGAR, TRIV

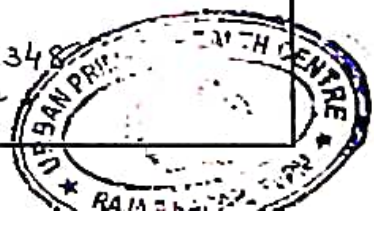


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

<b>Sl. No</b>	<b>Particulars</b>	<b>Details</b>
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	UPHC SECRTERIATE(RAJAJINAGAR)
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : Nebuliser Make : Truecheck Model :N8001 Serial No : N800115100002
4	Equipment ID/ Barcode	121407/0142953
5	Date of purchase/ Year of manufacture/Installation Date	01/06/2015
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	05/07/2024(Toll free)
9	Action taken	Checked and found motor and connector nozzle defective. Need to replace these spares for further checking and working condition of the equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE

13	Asset Value	1353/-
14	% Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	Checked and display and the main board defective. The equipment was installed on 01/06/2015 and covered upto 9+ years. Since the spares are not available in the market. Recommending the unit for condemnation
17	Name & Signature of CYRIX Authority	REHNA R 

\*Not mandatory


#Based on the period of life and value as per the BER guidelines

\* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Display and main board defective. So as per tender conditions this can be RBER

MANEESHA MOHAN M.R.  
Junior Consultant (Biomedical)  
National Health Mission  
Thiruvananthapuram


8-07-2024 

Signature of JC BM (NHM)

MANEESHA MOHAN M.R.  
Junior Consultant (Biomedical)  
National Health Mission  
Thiruvananthapuram



Date: 8-7-2024




Signature of  
Superintendent/Medical Officer (I/c)  
MEDICAL OFFICE  
APHC RAJANIGAS, TYPID



*Nehemiah*  
**SUB STOCK INDENT REGISTER**

Sl. No	Name of Drugs	Stock In Hand	Receipt	Issue	Balance	Initial
1	2	3			5	6
11/11	Received from main stock					
	Page 12: 27 from					
	Main stock register vol II	0	1		1	Clm
25/2/2015	Nebulizer is not working properly. Referred to NRIH of ficu.					
16/2/2015	Received from main stock page no: 29 from main stock register vol II	0	1	1	2	Siml

*Rama*

MEDICAL OFFICER  
 UPIC, RAIPUR, JHARKHAND

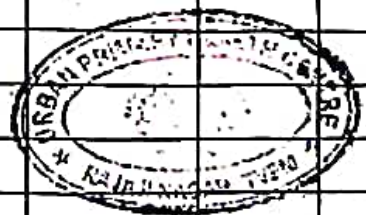

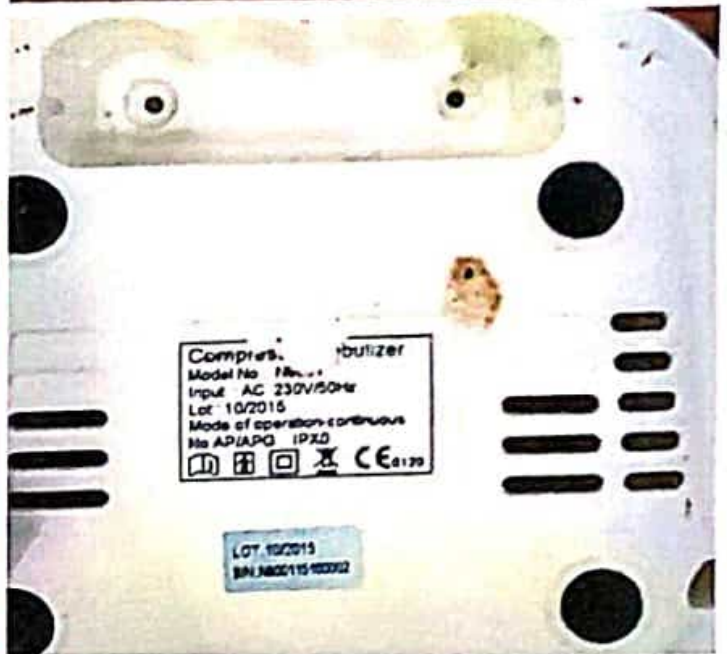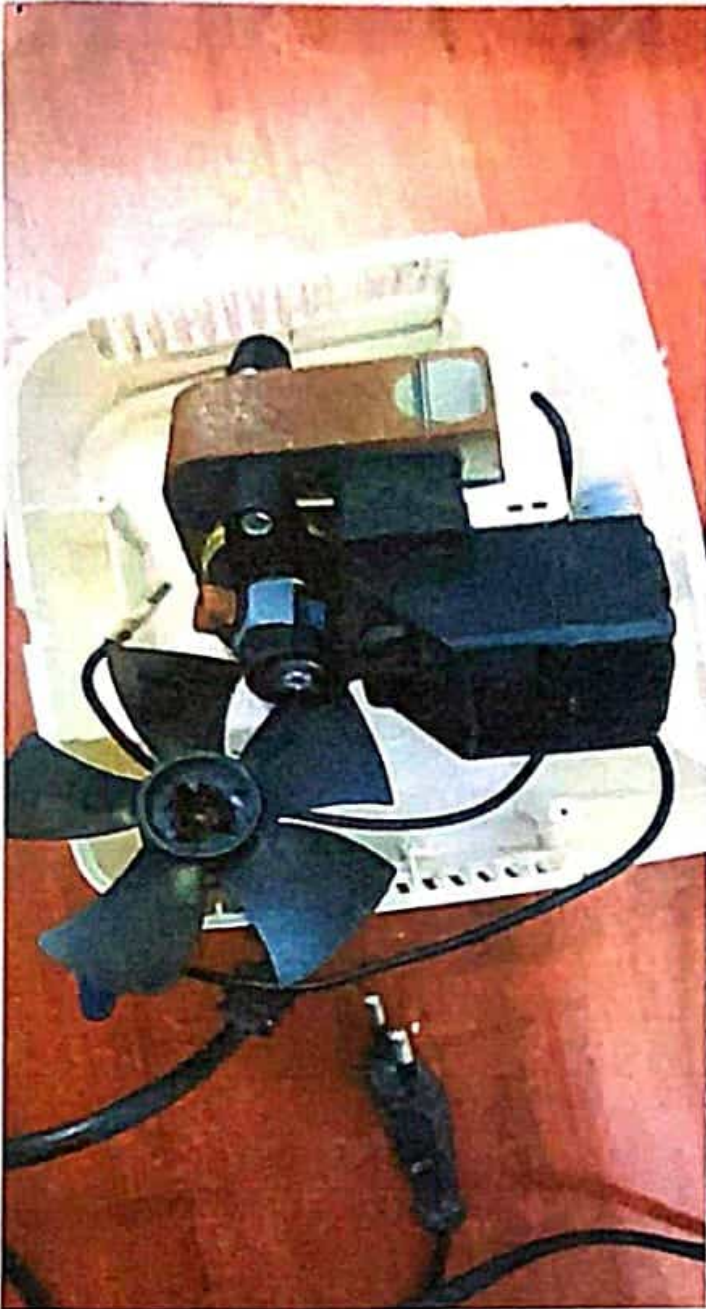

Compress. Inhalizer  
Model No. F80...  
Input AC 230V/50Hz  
Lot: 10/2015  
Mode of operation continuous  
No ADI/ADG IPX0

LOT 10/2015  
BIN/ABC/15/100012



*Reena*  
MEDICAL OFFICER  
UPHC, RAJAH NAGAR, T.P.M.