



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :

224193

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility W & C</p> <p>Address Thycaud, Thiruvananthapuram</p> <p>Ph : 7293749277</p>	<p>Call Registration Date : 2 - 7 - 2024</p> <p>Caller ID : 120458</p> <p>Date of Visit : 3 - 7 - 2024</p> <p>Asset No. : 0117055</p> <p>EQPT Name : BP Apparatus</p> <p>Manufacture Elko Model : mercury</p> <p>S. No. 528514 Dept. Ward T</p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : mercury spillage.

Action Taken : Checked the equipment and found mercury spillage. Identified BP glass rod and mercury tank defective. Need to replace these spares for further checking and working condition of the equipment.

Completed Date : 3-7-2024 Time : 9:45a.m Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.	NA	NA	NA	NA
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
Rehna R	3-7-2024	9.30a.m	9.45a.m

Customer Remark Completed Pending



Service Engineer Name : Rehna R
Signature : *Rehna*
Date : 3-7-2024
Contact Number : 9947239956

Customer Name : Nithya G S
Signature : *Nithya*
Date : 3/7/24
Contact Number : 9947268728
Designation : Nursing Officer
Hospital Seal : *Thycaud*


SUPERINTENDENT
Govt. W & C H. Thycaud
Thiruvananthapuram - 14

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	WOMEN AND CHILD HOSPITAL THIRUVANANTHAPURAM
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : BP Apparatus Make : Anita Industries Model : Elkometer Serial No : 528514
4	Equipment ID/ Barcode	120458/0117055
5	Date of purchase/ Year of manufacture/Installation Date	22/11/2022
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	02/07/2024(Toll free)
9	Action taken	Checked and found mercury spillage. Identified glass rod and control valve defective. Need to replace these spares for further checking and working condition of the equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE

13	Asset Value	1323/-
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found mercury spillage. Identified glass rod and control valve defective. Since the mercury is not available in the market. Recommending the unit for condemnation
17	Name & Signature of CYRIX Authority	REHNA R 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

glass rod defective, mercury spillage. So as per tender conditions, can be RBCP.

MANEESHA MOHAN M.R.
 Junior Consultant (Biomedical)
 National Health Mission
 Thiruvananthapuram


 10.07.2024
 Signature of JC BM (NHM)

Date:




 Signature of
 Superintendent/Medical Officer (i/c)
SUPERINTENDENT
 Govt. W & C Hospital Thycaud
 Thiruvananthapuram - 14

128


STOCK REGISTER OF

Name of Article

B.P apparatus

also p. 1



Date	No. and Qty of articles or bundles	From whom received or to whom issued	Receipt	Issued	Balance after each transaction	Amount of Balance	Remarks
16/10/2019	Brought forward	B.P apparatus Chemical for shop	1		(1)		
22/11/22		Received for Shiel 2 L.P - (Etkomul) Barcode - 0117055-50152004 - 0117055-501520515			(3)		



Carried over

Sankar

SUPERINTENDENT
 Govt. W & C Hospital, Thycapra
 Thiruvananthapuram - 14

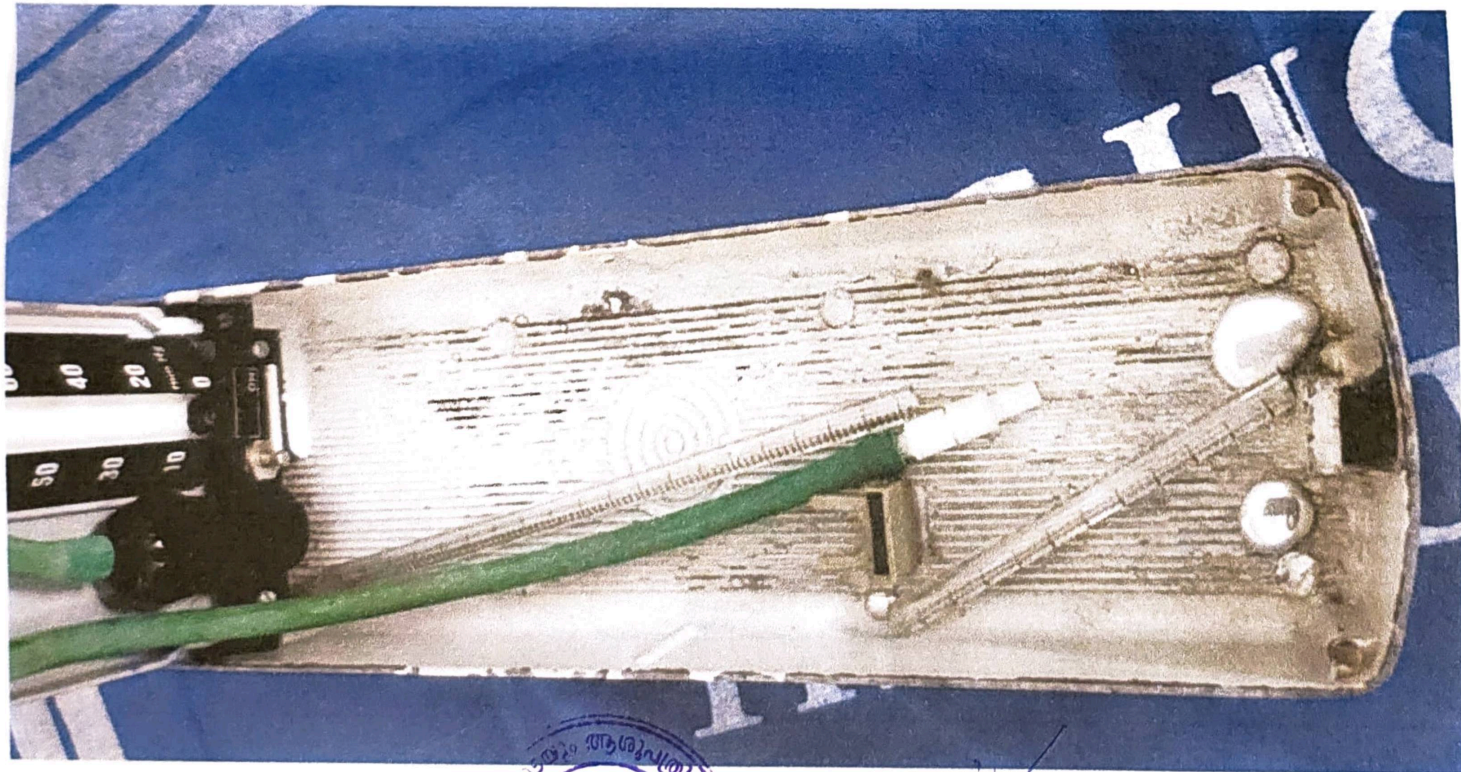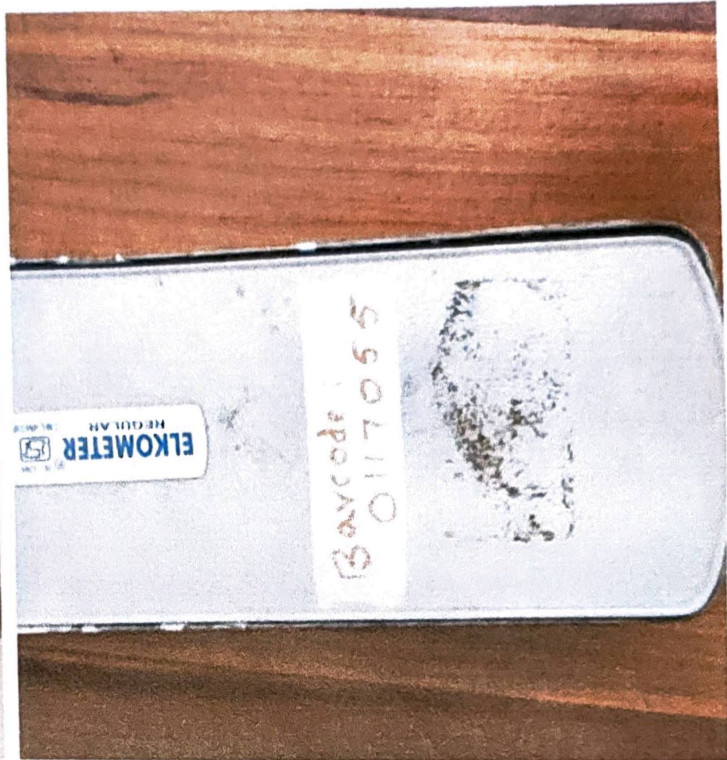

Sankar
SUPERINTENDENT
 Govt. W & C H. S. School, Thycaud
 Thiruvananthapuram - 14