



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 229567

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility	Taluk Hospital,	Call Registration Date :	03-06-2024
Address	North Paravur, Ernakulam (DE)	Caller ID :	114742
Ph :	09645126998	Date of Visit :	04-06-2024
		Asset No. :	0721565
		EQPT Name :	Suction Apparatus
		Manufacture	Monarch Model : MSI-R602
		S. No.	2019022 Dept. PP Unit.

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Suction Apparatus not working

Action Taken : checked the machine and found that motor, bottle, filter and tubings are defective.

Completed Date : 04-06-24 Time : 2:00 PM Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1. Motor	1 No.		
2. Bottle	2 Nos		
3. Filter and tubings	1 Each		
Cyrix Engineer		Date	Start Time
Jibin Thomas George		04-06-24	10:00 AM
			2:00 PM

Customer Remark Completed Pending

Service Engineer Name : Jibin Thomas
Signature : *Jibin Thomas*
Date : 04-06-24
Contact Number : 9047958051

Customer Name : *at*
Signature :
Date :
Contact Number :
Designation :
Hospital Seal :

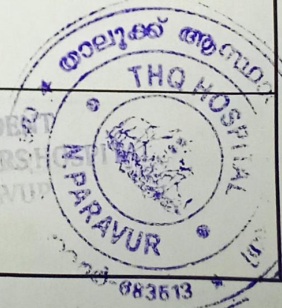


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	Ernakulam
2	Name of Hospital	TALUK HOSPITAL NORTH PARAVUR
3	Name of Equipment with Make, Model and Serial Number	Equipment: SUCTION APPARATUS Make : MONARCH Model : MSI-RGO2 Sr.no : NA
4	Equipment ID & Barcode	114742 & 0721565
5	Date of purchase / Year of manufacture /Installation Date	29-03-2019
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	03-06-2024 (Toll Free)
9	Action taken	Checked the machine and found that motor, bottle, filter and tubings are defective.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	MOTOR-1NO-RS.4650 BOTTLE WITH LID-2NOS-RS.3250 FILTER-1NO-RS.230 TUBINGS-1NO-RS.300 TOTAL AMOUNT-RS.9947

13	Asset Value	Rs.9,900
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	100.47%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found that motor, bottle, filter and tubings are defective. Enquired the spare and spare cost for repairing is 100.47% of the equipment asset value. Equipment installed on 29-03-2019 and the machine outlived 5+years. So recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	JIBIN THOMAS GEORGE 

*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Installation date of asset is 17/8/17, submitted BER after 30 days. As per the quotation attached the repair cost is more than the asset value
Rs. 9900/-


Devidy Consultant BME
24/7/24
Signature of JC BM (NHM)

CONSULTANT Engineer
National Health Mission (NHM)
Aryyakkal

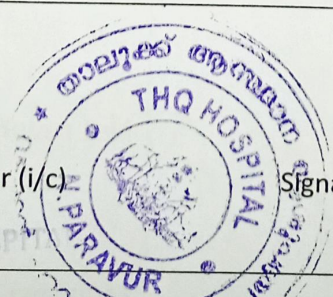

Superintendent / Medical Officer (i/c)  Signature of seal

Date

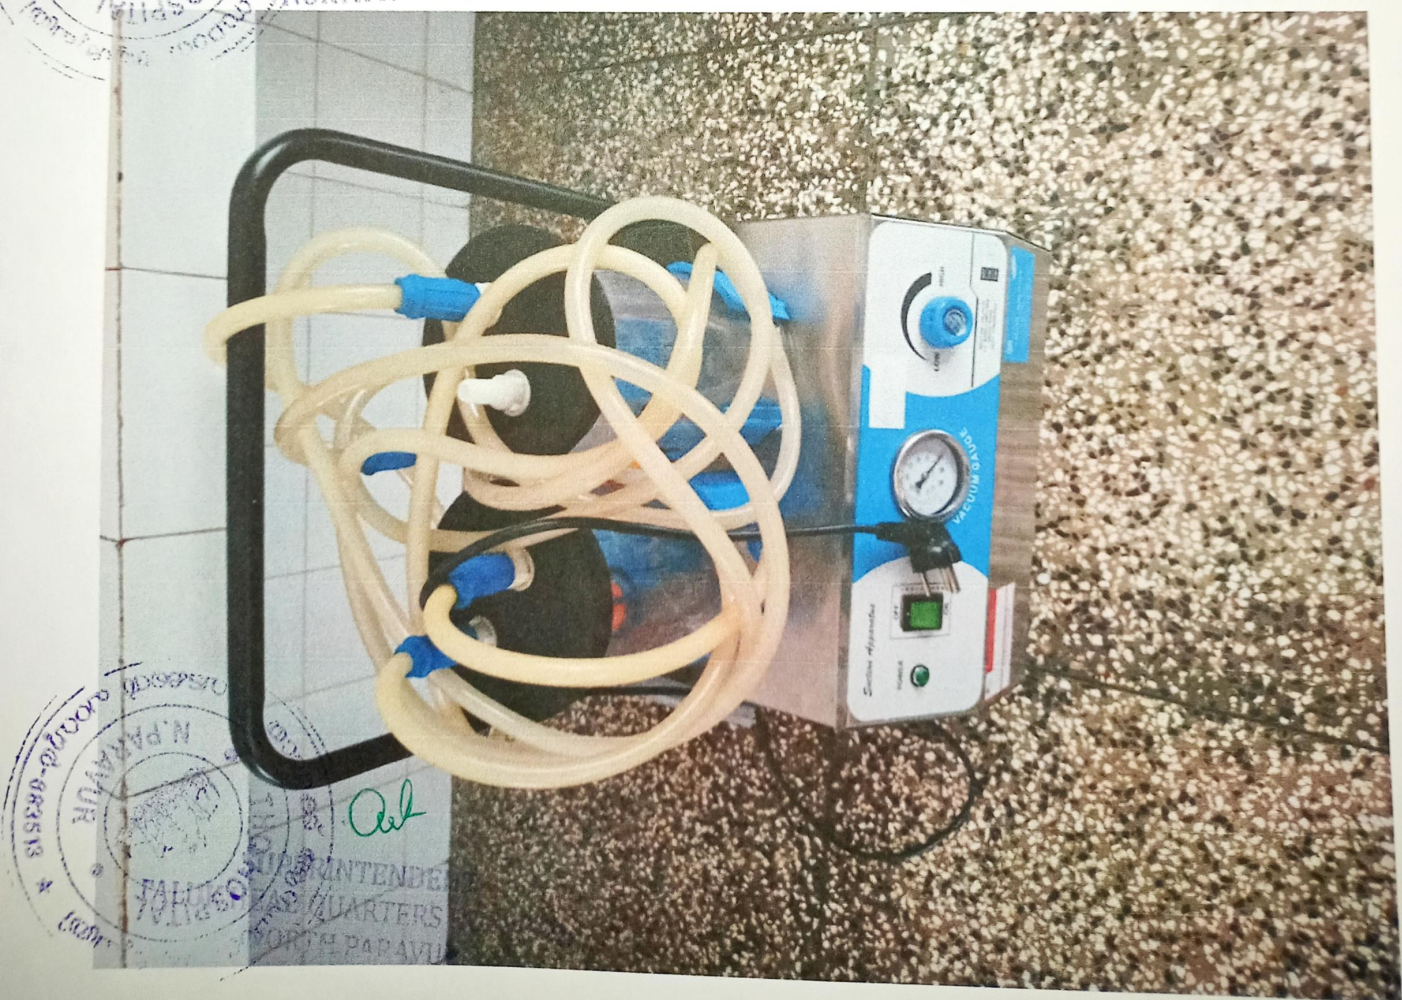



STOCK REGISTER

Item 220 Suction Apparatus. (1)

Date	Invoice/ Voucher No.	Received from or issued to	Cost	Receipt	Issue	Balance	Remarks	Intls.
29/3/19		model RC1 - 02		181			marked.	
		value - 22176.00					original value 19800.	
		issued on		29/3/19			from store	
29/6/23		Pr.out to mm					1 <u>NFI</u>	




 SUPERINTENDENT
 TALUK HEAD QUARTERS HOSPITAL
 NORTH PARAVUR



CLOUD99

Office : 97444 73043

Service : 97444 73243

Sales and service of all kinds of medical equipments

Room No: 22, First Floor, CSI Golden Jubilee Complex,

Behind Shastri Road Waiting Shed, Kottayam-686001

Email: cloud99biotech@gmail.com

QUOTATION

Date: 10/06/2024

To,

TH Paravur

ERNAKULAM

Dear Sir

We are pleased to submit a quotation for **TH, Paravur** for Suction Apparatus. Bar code is **0721565**.

SL No	ITEM NAME	PRICE PER UNIT	GST	PRICE INCLUDING GST
1	MOTOR	4650	18%	5487
2	BOTTLE WITH LID - 2 NOS	3250	18%	3835
3	FILTER	230	18%	271
4	TUBINGS	300	18%	354
	TOTAL			9947

Terms & Conditions

1. Taxes: GST @ 18 % inclusive
2. Payment Terms: 100% advance payment
3. Quotation validity: 15 days from date of quotation


We hope you will find our rates are competitive and wait for your valued order.

Thanking you,

Yours Faithfully

FOR CLOUD99 BIOTECH

AUTHORIZED SIGNATORY

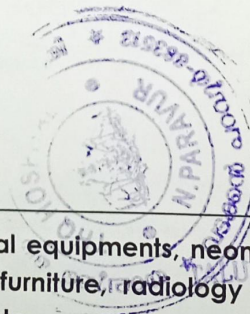

We deal with sales and service of all kinds of hospital equipments, neonatal equipments, laboratory equipments, dental equipments, suction, hospital furniture, radiology equipments, physiotherapy equipments, all type of autoclaves, ICU equipments, etc.