



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 205025

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>pbc chadaya mangalam</u></p> <p>Address <u>chadaya mangalam</u> <u>kollam</u></p> <p>Ph : <u>94 95 43 14 60</u></p>	<p>Call Registration Date : <u>21/6/2024</u></p> <p>Caller ID : <u>118515</u></p> <p>Date of Visit : <u>22/6/2024</u></p> <p>Asset No. : <u>0242453</u></p> <p>EQPT Name : <u>Nebuliser</u></p> <p>Manufacture <u>lifeline</u> Model : <u>Alpha</u></p> <p>S. No. <u>NA</u> Dept. <u>OP</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Nebuliser machine not getting on

Action Taken : Checked the nebuliser and found that the motor defective and piston damaged. Need to replace these spares for further checking and working condition of this equipment

Completed Date : 22/6/2024 Time : 4:00 PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time

Customer Remark Completed Pending

<p>Service Engineer Name : <u>Rajeshlal A S</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>22/6/2024</u></p> <p>Contact Number : <u>7593847128</u></p>	<p>Customer Name : <u>Asif Khan - 2</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>22/6/2024</u></p> <p>Contact Number : <u>9495431460</u></p> <p>Designation : <u>Senior A/c</u></p> <p>Hospital Seal :</p>
--	--




Handwritten signature and stamp of Medical Officer in Charge, Family Health Center, Chadayamangalam - 591334

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	Kollam
2	Name of Hospital	Phc chadayamangalam
3	Name of Equipment with Make, Model and Serial Number	NEBULIZER Make : Life Line Model : ALPHA SI no: Nil
4	Equipment ID & Barcode	Barcode : 0242453 / Ticket id : 118515
5	Date of purchase / Year of manufacture /Installation Date	16-05-2018
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	21-06-2024
9	Action taken	Checked the machine found that the Nebulizer motor and piston are damaged. Need to replace these spares for further checking &working condition of these equipment
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not Recommended for Repair
12	Cost of spares (specify parts and cost)	NA


13	Asset Value	Rs. 2162/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report attached
16	Reasons for recommending the equipment as BER	Checked the machine and found that the nebulizer motor and piston are defective, enquired for spares in the market but spare are not available. Equipment is installed on 16-05-2018 and aged upto 6+ year. So we are recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	RAKESH R 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Fully damaged and recommended for Beyond economic repair


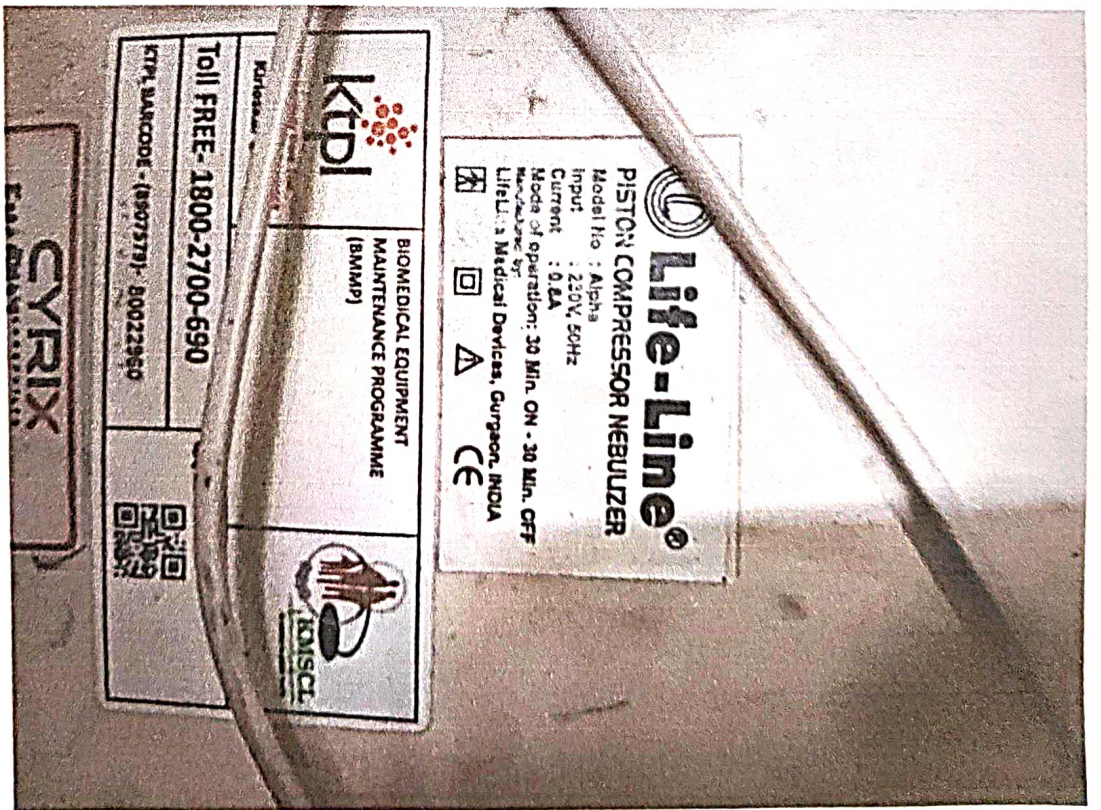

09/07/24

Signature of JC BM (NHM)
ABMO
NHM, KOLLAM

Date 8/7/2024




Signature of Superintendent/
Medical Officer in Charge
Family Health Center
Chadayamangalam- 691534



[Handwritten signature]

Medical Officer in Charge
Family Health Center
Chadeyungulam- 691534

