



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 223697

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility : <u>CHC Velland</u>	Call Registration Date : <u>21/06/2024</u>
Address : <u>Trivandrum</u>	Caller ID : <u>118465</u>
Ph : <u>7012424977</u>	Date of Visit : <u>26/06/2024</u>
	Asset No. : <u>0130619</u>
	EQPT Name : <u>UPS</u>
	Manufacture : <u>NA</u> Model : <u>NA</u>
	S. No. : <u>NA</u> Dept. : <u>Laboratory</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : checked and found that the inverter PCB, control PCB and 12V 7AH battery defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spare with vendors.

Completed Date : 26/06/24 Time : 11:30 AM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2. <u>NA</u>	<u>NA</u>	<u>NA</u>	<u>NA</u>
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Midhun . SM</u>	<u>26/06/24</u>	<u>10:30 AM</u>	<u>11:30 AM</u>

Customer Remark Completed Pending



Service Engineer Name : midhun . sm
Signature : Midhun
Date : 26/06/2024
Contact Number : 9074167987

Customer Name : Bodhi
Signature : [Signature]
Date : 26/6/2024
Contact Number : 944614903
Designation : Health Officer
Hospital Seal :


Medical Officer In-Charge
Community Health Centre Velland
Thiruvananthapuram-695543

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	CHC VELLANAD
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : UPS 1KV Make : Asia Power Model : AP1050+ Serial No : UV060714AA000634
4	Equipment ID/ Barcode	118465/0130619
5	Date of purchase/ Year of manufacture/Installation Date	15/03/2017
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	21/06/2024
9	Action taken	Checked and found that the inverter PCB, Control PCB and 12v 7Ah battery defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spare with vendor.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	1KVA 24V Inverter PCB - 4130/- 1KVA Control PCB - 2950/- 12v 7 Ah Battery (2Nos) - 2176/- Total=9256/-

13	Asset Value	11000/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	84.1%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT AND VENDOR REFERENCE QUOTATION ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found that the inverter PCB, Control PCB and 12v 7Ah battery defective. The unit was installed on 15/03/2017 and covered upto 7+ years. The repairing cost is 84.1%. As per the tender clause 5.3.14.1 Both criteria met. So recommending the unit for condemnation.
17	Name & Signature of CYRIX Authority	MIDHUN BM 


*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Inverter PCB, Control PCB and battery defective.
So as per tender condition can be RBER.

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


20.07.2024
Signature of JC BM (NHM)

Date:




Officer In-Charge
Superintendent's Office
Community Health Centre Vellanad
Thiruvananthapuram (IC)
995543

HEMATOLOGY

ANALYSER. 3 PARTS

(PE-6000) 58

B.C(8004)8907579 - 70012411

1) HEMATOLOGY ANALYSER. Received from KMCL
 15/3/17. Invoice No RDP/1969/16-13 KMCL from
 Rapid Diagnostics Pvt Ltd TIN No. 3210101829.
 Rate of 2,25,645/- Master Register Vol I
 Page No. 63.

2 Hematology Analyser. A6006161200236EH
 UPS with back up
 Diluent 20L FOR PE 6.
 Lyse 500ML FOR PE 6
 Lyse 200ML FOR PE 60 Hematology Analyser - PE-6000
 RINSE 10 L FOR PE 6. Not working. Service Engineer
 RINSE 1 L FOR PE 6000 Reconnect for condensation.
 EZ cleaner 100ml for probe clean 100ml for

16-8-17

14/1/2023 provided standby machine and taken the Rapid machine MINDRAY

11/3/2022 Haematology Analyser Received from KMCL 11/3/22
 Invoice. No. DM/1090/21-22. Deep meditech Pvt. Ltd.
 (MEDITECH) GSTIN - 32AADCK4029M1ZK Gidya
 Order No - 50/898/22-22/ST

Rate of. 1,69,920 - (Block Fund) HMC
 Haematology Analyser (3 part) - 1 (MINDRAY)
 Model 215 / Shenzhen mindray
 TL - 10001141

Diluent 20L - 1 set.
 202111002 07-9/11/23

Lyse (500) - 1 set
 2021101401 09-10/10/23

Dish clean 1/2 5ml - 1 set
 22020206 08-30/1/23

UPS 1kVA online
 900012105110327

Page No. 64 of Medical Officer In-Charge
 Community Health Centre Vellana
 Thiruvananthapuram-695013

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 13/07/2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN : 32CGUPM9450L1ZN

1KVA ONLINE UPS SERVICE PROPOSAL

TO,
CYRIX HEALTHCARE PVT. LTD
Barcode: 0130192
Ticket ID: 113214

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST	TOTAL PRICE IN INR
1	1KVA 24V INVERTER PCB	1	3500.00	3500.00	18	4130.00
2	1KVA CONTROL PCB	1	2500.00	2500.00	18	2950.00
3	12v 7Ah Battery	2	850.00	1700.00	28	2176.00
PAYABLE AMOUNT						9256.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20%After installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares, 28%@Battery
4. Installation; Our scope.

Please arrange to release the PO at our above address

Bank name :HDFC

Account no:50200082743176

IFSC Code:HDFC0004083

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query.

Thank you, Sincerely,
BHAGATH MOHAN





REGARDING QUOTATION FOR UPS-CHC ANCHUTENGU (0130192 0130178)

2 messages

Kasyep P V <kasyepcyrix@gmail.com>

Thu, 18 Jul 2024 at 10:02 pm

To: aionbackups12@gmail.com <aionbackups12@gmail.com>

Dear sir,

Kindly provide the service quotation for the 1 KV UPS at CHC Anchuthengu, Trivandrum

--

Thanks & Regards,

KASYEP PV

District Incharge , Trivandrum

CYRIX HEALTHCARE Pvt.Ltd

KLBEMP

Ph : +91 7593847134

kasyepcyrix@gmail.com

Bhagath Mohan <aionbackups12@gmail.com>

Thu, 18 Jul 2024 at 11:19 pm

To: Kasyep P V <kasyepcyrix@gmail.com>



Received your mail.

Thanks & Regards

Bhagath Mohan

PH:-8921950217

[Quoted text hidden]

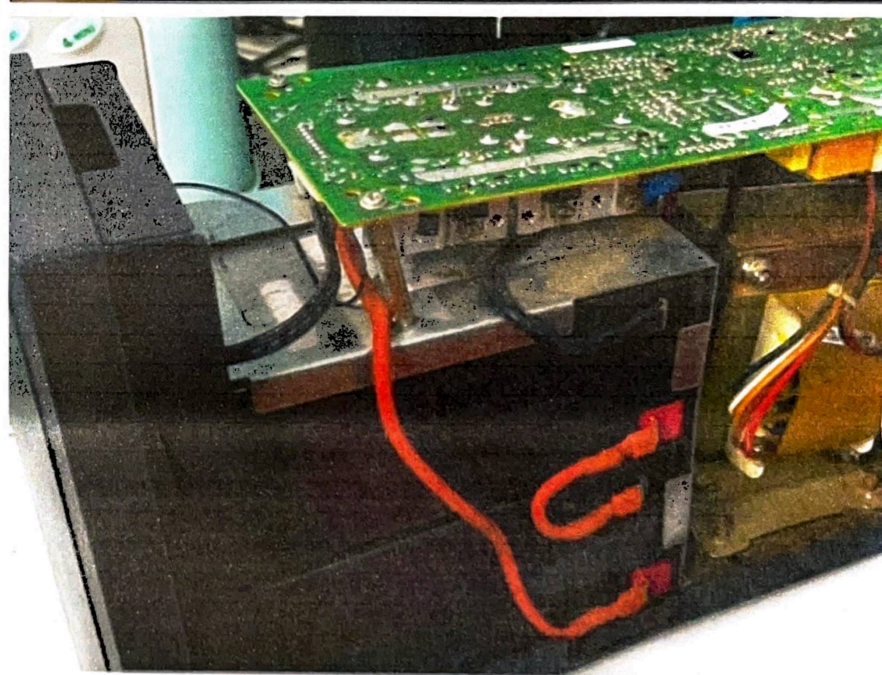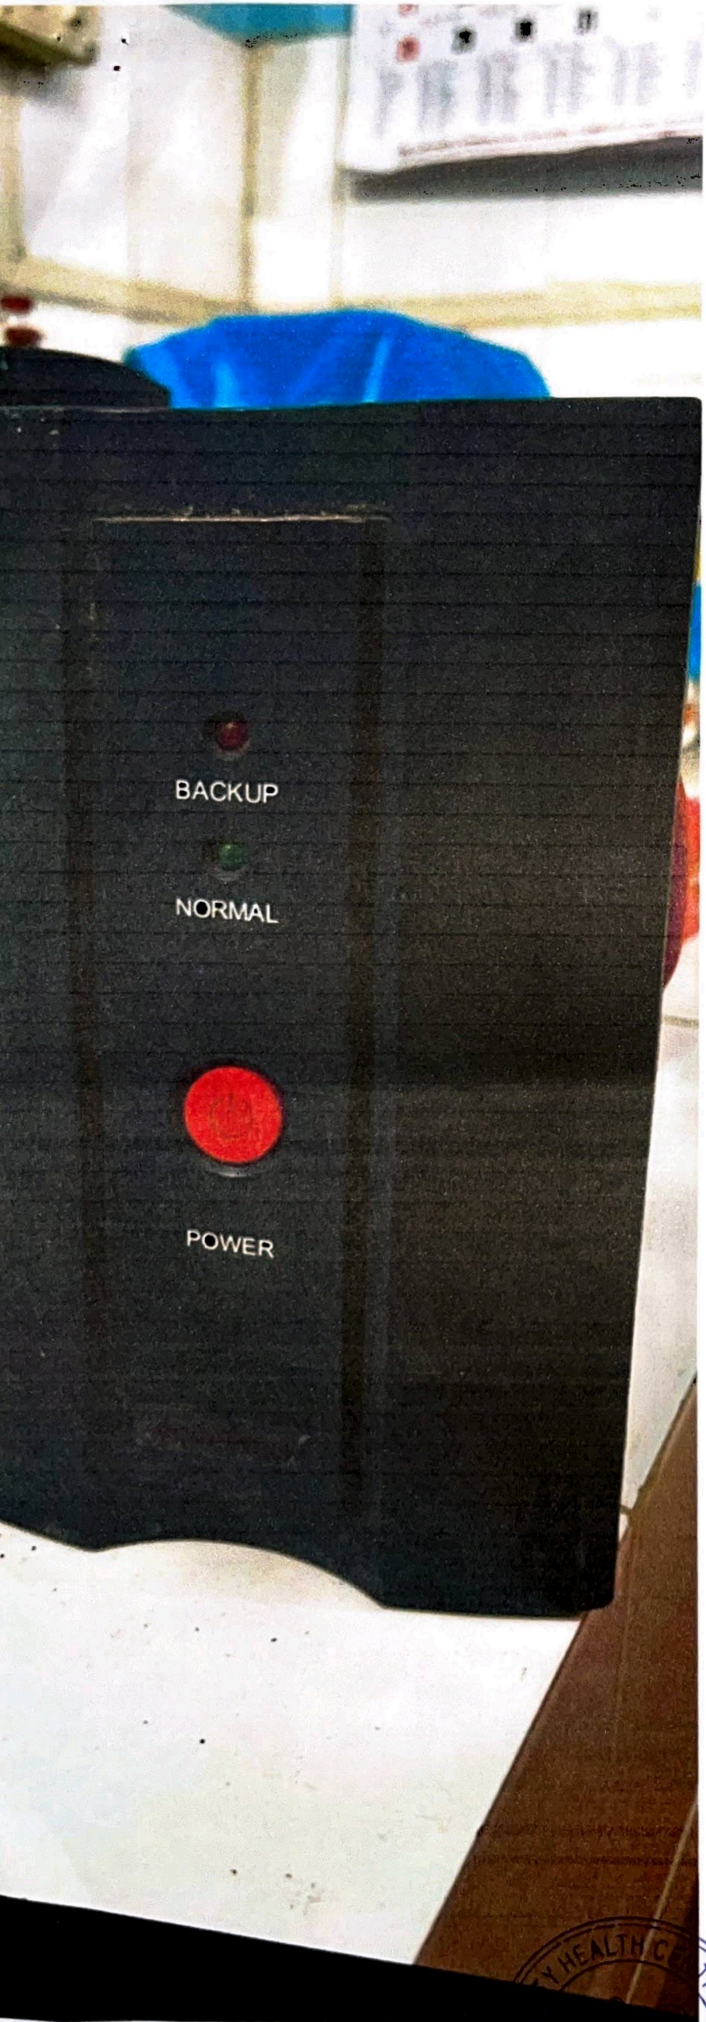

Medical Officer In Charge
Community Health Centre Vellanoor
Thiruvananthapuram-695543