

No Negotiation needed



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 228361

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

| | |
|-------------------------------|---|
| Health Facility : F.H.C. Anad | Call Registration Date : 21/06/2024 |
| Address : Trivandrum | Caller ID : 118368 |
| Ph : 9895758970 | Date of Visit : 25/06/2024 |
| | Asset No. : 0140776 |
| | EQPT Name : pharmacy Refrigerator |
| | Manufacture : Videocor Model : VZ205 |
| | S. No. : NA Dept. : pain and palliative |

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : not working

Action Taken : checked and found that the bearing, compressor filter and capillary defective. need to replace these spare for filter checking and working condition of the equipment. Enquired the spares with vendor.

Completed Date : 25/06/24. Time : 10:00 AM Spare Required


Spare Replaced Requested

| Description | Qty. | Part Number | PR Number |
|-------------|------|-------------|-----------|
| 1. | | | |
| 2. NA | NA | NA | NA |
| 3. | | | |

| Cyrix Engineer | Date | Start Time | End Time |
|----------------|----------|------------|----------|
| midhun . BM | 25/06/24 | 9.00 AM | 10.00 AM |

Customer Remark Completed Pending

Service Engineer Name : midhun . BM
Signature : *[Signature]*
Date : 25/06/2024
Contact Number : 9074167987



Customer Name : *[Signature]*
Signature : *[Signature]*
Date : 25/6/2024
Contact Number : 9895758970
Designation : Nursing officer grade 1
Hospital Seal : *[Seal]*


Medical Officer in-charge
Community Health Centre
9895758970

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

| Sl. No | Particulars | Details |
|--------|--|--|
| 1 | Name of District | THIRUVANANTHAPURAM |
| 2 | Name of Hospital | PHC ANAD |
| 3 | Name of Equipment with Make, Model and Serial Number | Equipment Name : Pharmacy refrigerator Make : Videocon Model : VZ205 Serial No : NA |
| 4 | Equipment ID/ Barcode | 118368/0140776 |
| 5 | Date of purchase/ Year of manufacture/Installation Date | 20/05/2017 |
| 6 | Warranty details (Yes/No) | No Warranty |
| 7 | *AMC/ CAMC Period agreed at the time of purchase | No CAMC/AMC |
| 8 | Date of breakdown (Date of registration of complaint through email/ Toll free) | 21/06/2024 |
| 9 | Action taken | Checked and found that the beading, compressor filter and capillary defective. Need to replace these spare for further checking and working condition of the equipment. Enquired the spares with vendor. |
| 10 | Present status of the equipment (Fully damaged / partially damaged) | FULLY DAMAGED |
| 11 | Recommendations for repair (required service details) | NOT RECOMMENDING FOR REPAIR |
| 12 | Cost of spares (specify parts and cost) | Compressor -4100 Gas charging, filter and capillary -1800/- Door beading -950/- Transportation - 2200/- TOTAL - 9050/- |

| | | |
|----|--|--|
| 13 | Asset Value | 13100/- |
| 14 | * Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value | 69% |
| 15 | Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) | CYRIX SERVICE REPORT AND VENDOR QUOTATION ATTACHED |
| 16 | Reasons for recommending the equipment as BER | Checked and found that the beading, compressor, filter and capillary defective. The unit was installed on 20/5/2017 and covered up to 7 + years. The repairing cost is 69%. As per the tender clause 5.3.14.1 both criteria met. So recommended the unit for condemnation. |
| 17 | Name & Signature of CYRIX Authority | MIDHUN BM  |


*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Verified the estimate, since all the major parts are damaged and estimate is above 69% this can be


MANEESHA MOHAN M.R.
 Junior Consultant (Biomedical)
 National Health Mission
 Thiruvananthapuram


 26-07-2024
 Signature of JC BM (NHM)

Date:






 Signature of
 Superintendent/Medical Officer (i/c)
 Medical Officer in-charge
 Family Health Centre

Anad-695 541

REFRIGERATOR

| DATE | DESCRIPTION | RECEIPT | ISSUE | BALANCE | INRM |
|-----------|--|---------|---------------------------|---------|------|
| 23/3/17 | Form Register of equipments & instruments | | book NO: I Page no: 20 | | |
| | Crocheji double door Amt: 9850/- | 1 Nos | | 1 Nos | 2 |
| 20/5/17 | Videocass Refrigerator Amt: 13900/- | 1 Nos | | 2 Nos | 2 |
| 16/2/2020 | Form register of equipments & instruments book no: II page no: 62 Amt: 14700/- | | | | |
| | Crocheji Refrigerator 205 TAF (For palliative insulin stock) 3.2, C.L.S (Blue) | 1 Nos | | 3 Nos | 2 |




 Medical Officer in charge
 Family Health Centre
 And-695 541



PERFECT AIR CONDITIONER

Chemmathoor near private bus stand
punalur, contact number: 9562185059
, Kollam, Kerala, 691305

QUOTATION

Quotation No. : 753
Quotation Date : 22/07/2024
Expiry Date : 29/07/2024

BILL TO

Cyrix Health Care

| S.NO. | ITEMS/SERVICES | QTY. | RATE | AMOUNT |
|-------|---|-------|-------|--------|
| 1 | COMPRESSOR CHANGE | 1 PCS | 4,100 | 4,100 |
| 2 | GAS CHARGING & FILTER CHANGE & CAPILLARY CHANGE | 1 PCS | 1,800 | 1,800 |
| 3 | DOOR BEADING CHANGE | 1 PCS | 950 | 950 |
| 4 | TRANSPORTATION CHARGE | 1 PCS | 2,200 | 2,200 |

SUBTOTAL

4

₹ 9,050

NOTES

PHC ANAD
Pharmacy refrigerator
Barcode: 0140776
Ticket id: 118368
Make :Videocon
Model : VZ205

TAXABLE AMOUNT

₹ 9,050

TOTAL AMOUNT

₹ 9,050

Total Amount (in words)
Nine Thousand Fifty Rupees

BANK DETAILS



Name: ANIJA A J
IFSC Code: SBIN0070779
Account No: 67261447806
Bank: State Bank of India ,PSBADOOR



ANIJA A J
Medical Officer in-charge
Punalur Health Centre



Authorized Signature for
PERFECT AIR CONDITIONER

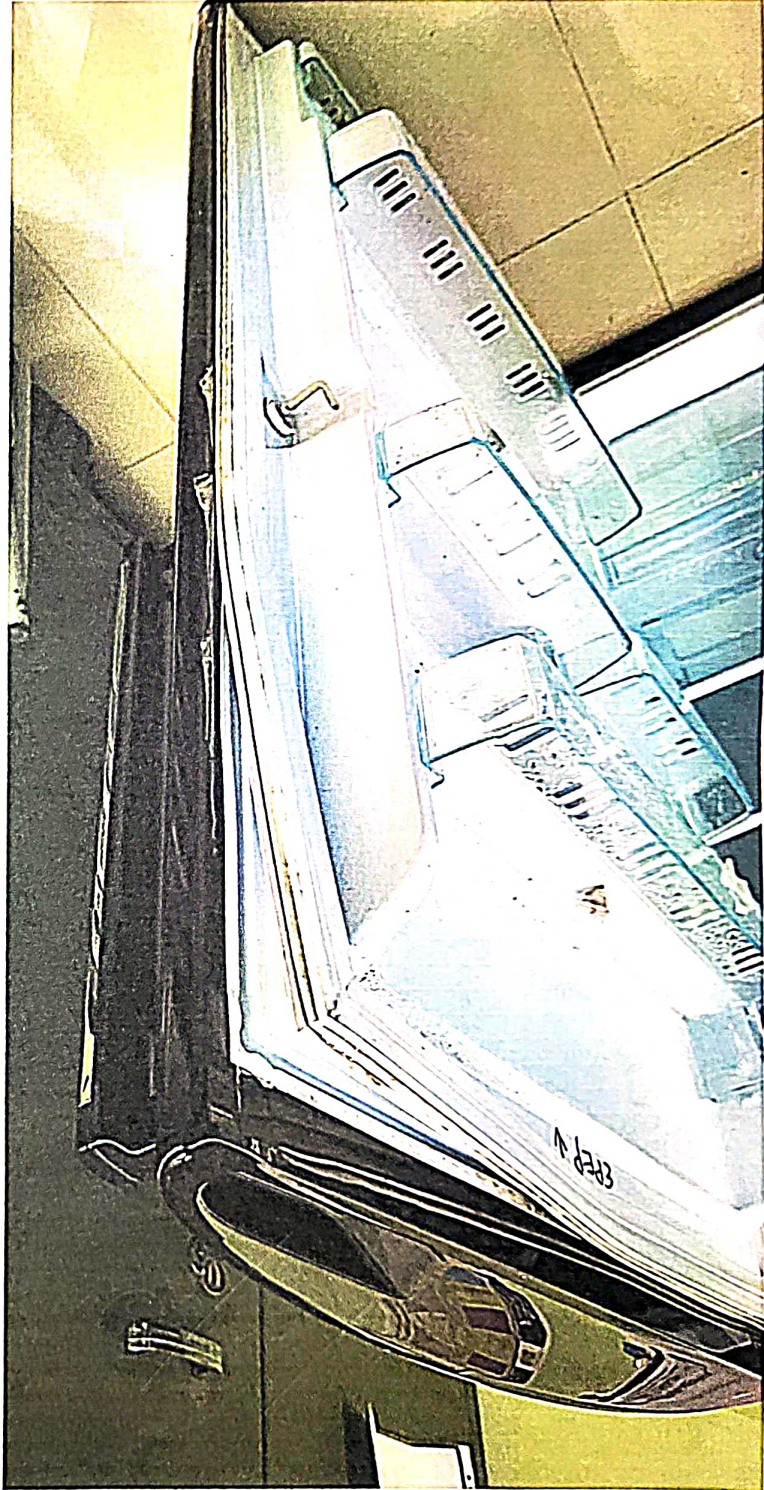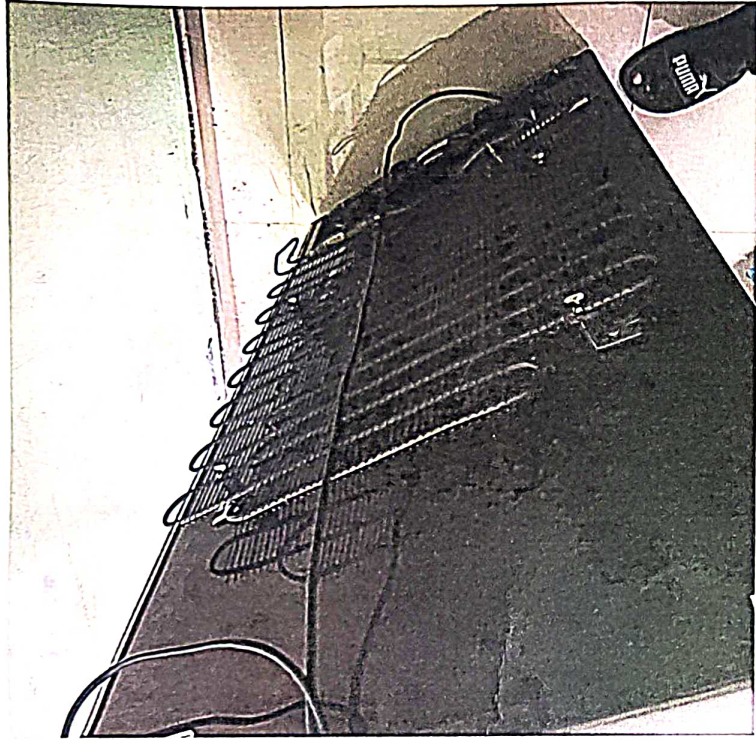

180 9881 3888 (continued on p. 174/85/074)
CYRIX
FICHAIRES...
REFRIGERATOR
Due: 15-05-24
Due: 14-05-25

CYRIX MEDICAL EQUIPMENT MAINTENANCE PROGRAMME (SERV)
TOLL FREE NO: 1800 - 425-7669
BAR CODE - (8004-890615225)
0140776



Pat

Medical Out-patient Incharge
Family Health Centre
Anand-009 101