



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 170642

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>CPC VELIYANAD</u></p> <p>Address</p> <p style="padding-left: 40px;">DIST: <u>ALAPPUZHA</u></p> <p>Ph : <u>9495744518</u></p>	<p>Call Registration Date : <u>18/7/24</u></p> <p>Caller ID : <u>123843</u></p> <p>Date of Visit : <u>19/7/24</u></p> <p>Asset No. : <u>0430507</u></p> <p>EQPT Name : <u>(DELTA) UPS</u></p> <p>Manufacture <u>DELTA</u> Model : <u>UPA102V21DO</u></p> <p>S. No. <u>44180950346</u> Dept. <u>LAB</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Battery issue

Action Taken : On checking found that batteries are faulty need to replace batteries (12V, 7AH) 2 nos for further checking

Completed Date : 19/7/24 Time : 1:00 PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Michbus raj R</u>	<u>19/7/24</u>	<u>12:00 PM</u>	<u>1:00 PM</u>

Customer Remark Completed Pending



Service Engineer Name : Michbus raj R

Signature : [Signature]

Date : 19/7/24

Contact Number : 9072522056

Customer Name : Shajin P. A

Signature : [Signature]

Date :

Contact Number : 9497780827

Designation : Laboratory Technician

Hospital Seal :



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 170650

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>CHC VEHYANAD</u></p> <p>Address</p> <p><u>DIST. ALAPPUZHA</u></p> <p>Ph : <u>9495744518</u></p>	<p>Call Registration Date : <u>18/7/24</u></p> <p>Caller ID : <u>123843</u></p> <p>Date of Visit : <u>19/7/24</u></p> <p>Asset No. : <u>0430507</u></p> <p>EQPT Name : <u>UPS</u></p> <p>Manufacture <u>DELTA</u> Model : <u>VPA102V21</u> PBO</p> <p>S. No. <u>441809509346</u> Dept. <u>LAB</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Battery issue

Action Taken : Check the machine and found that the 24 VDC Inverter PCB and battery 12V 7AH are defective Enquired spare with the OEM

Completed Date : 25/7/24 Time : 3:00PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Midhun raj R</u>	<u>25/7/24</u>	<u>2:00PM</u>	<u>3:00PM</u>

<p>Service Engineer Name : <u>Midhun raj R</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>25/7/24</u></p> <p>Contact Number : <u>9072522056</u></p>	<p>Customer Name : <u>Shajino P-A</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>25/7/24</u></p> <p>Contact Number : <u>9497780823</u></p> <p>Designation : <u>Laboratory Technician</u></p> <p>Hospital Seal : <u>[Seal]</u></p>
---	---




MEDICAL OFFICER IN-CHARGE
Community Health Centre
Velluvannur

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	ALAPPUZHA
2	Name of Hospital	CHC VELIYANAD
3	Name of Equipment with Make, Model and Serial Number	UPS MACHINE MAKE :- DELTA MODEL :- VX 1000 VA SN :- 441B09509346
4	Equipment ID & Barcode	123843 & 0430507
5	Date of purchase / Year of manufacture /Installation Date	14/01/2019
6	Warranty details (Yes/No)	NO WARRANTY
7	*AMC/ CAMC Period agreed at the time of purchase	NO AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	18/07/2024
9	Action taken	Check the machine and found that the 24VDC Inverter PCB and Battery 12V,7Ah are defective. Enquired spare with the Vendor.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not Recommended For Repair
12	Cost of spares (specify parts and cost)	24V DC INVERTER PCB = 2596 <u>12V, 7AH SLA BATTERY (2) = 2176</u> TOTAL = 4772


13	Asset Value	RS - 4500/-
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	106%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report and Spare Quotation attached
16	Reasons for recommending the equipment as BER	Check the machine and found that the 24VDC Inverter PCB and Battery 12V,7Ah are defective. The equipment was installed on 14/01/2019 aged up to 5 Years and 6 Months. Repair cost of the equipment is 106%. Both criteria met as per the tender clause 5.3.14.1 So we are recommending the equipment as BER.
17	Name & Signature of CYRIX Authority	MIDHUN RAJ R 



*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Recommended for BER


 08/08/24
 JYOTHISH THOMAS
 Consultant (Biomedical Engineering)
 NHM ALAPPUZHA
 Signature of JC BM (NHM)


<p>Date</p>	<p> Seal</p> <p> Signature of Superintendent / Medical Officer (i/c) Community Health Centre Vellayanad</p>
-------------	--




HAEMATOLOGY ANALYZER 35

Date	Content	Received	Issued / Balance
	<u>AUTOMATED HAEMATOLOGY 3-PART ANALYZER</u>		
12/4/19	Received from Store I No. 01819-014424/18-19 dt- 11/1/2019. from PNC Mutter Installed on 16/4/19 Order No 97A/19 dt- 12/4/19	1	

- (1) Automated Haematology 3 part-
Differential Analyzer SI No. RJ-8B
127231
No.
- (2) Delts-1KVA UPS System IP- }
Input 230v output Mode Vx1000V } 1 Nos
- SI No. - 4418095093AC
- (3) Power Cord - 1 Nos.
Main Stock Reg Page No: 98




 NERC OFFICER IN CHARGE
 Community Health Centre
 Veliyanad

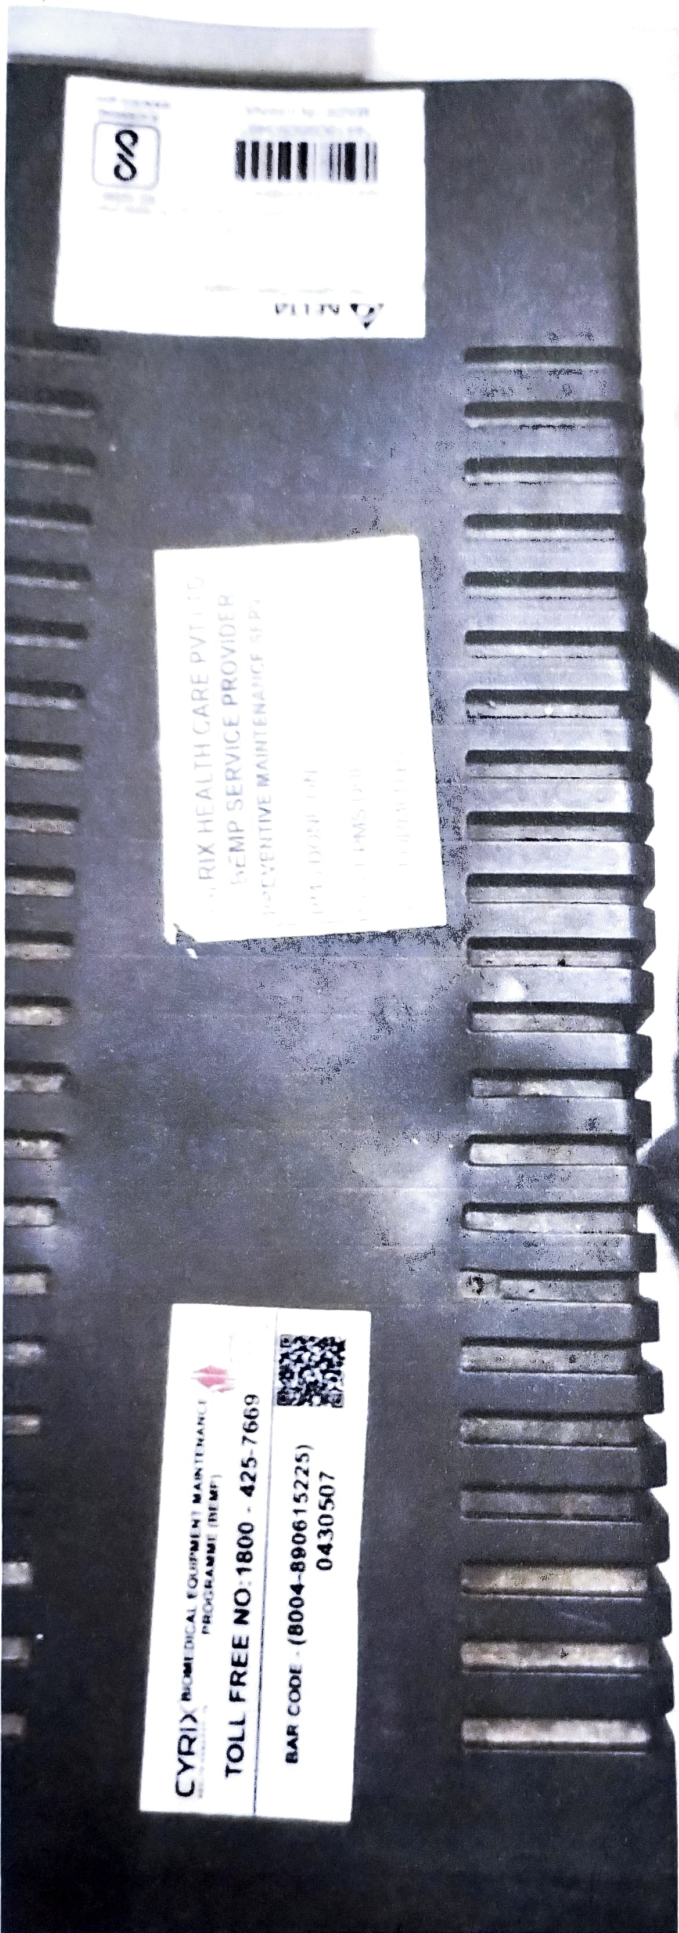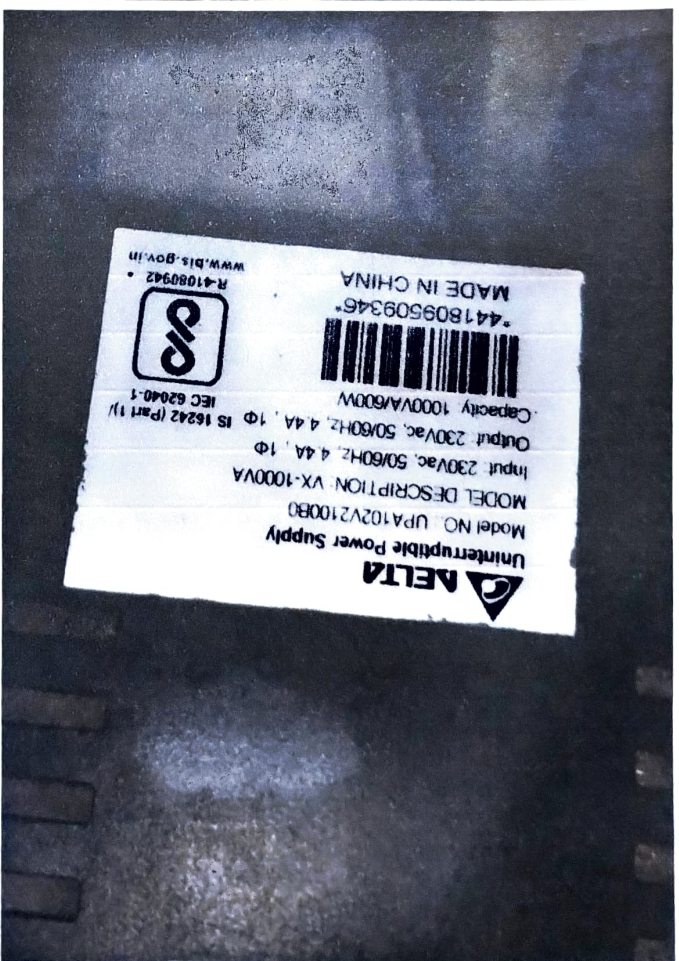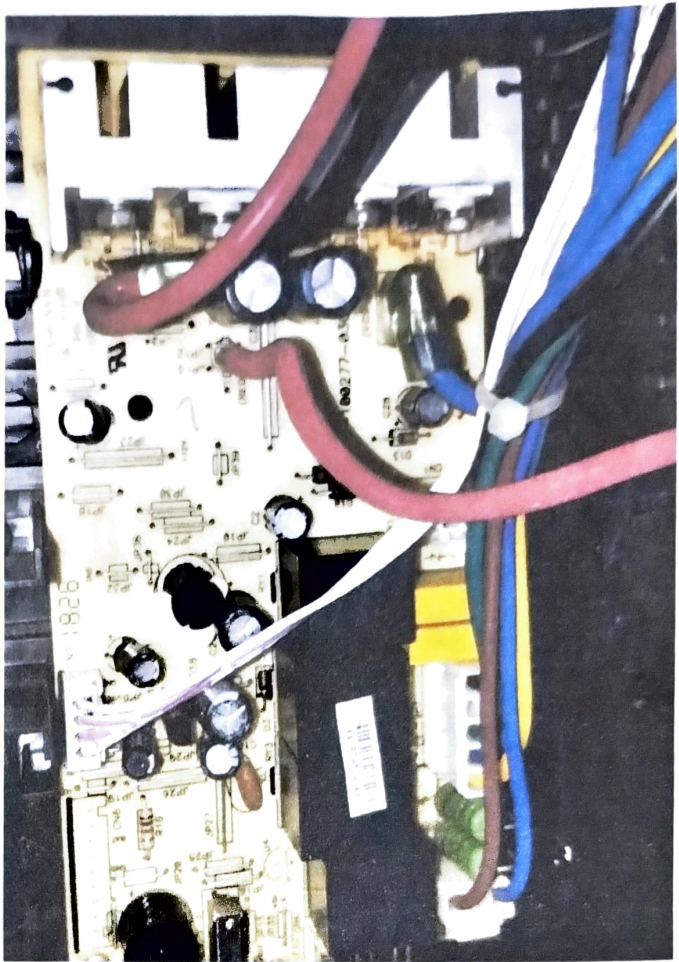

Medical Dept. ...
 ... only ...
 ...

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 25/07/2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN: 32CGUPM9450L1ZN

1KVA DELTA UPS SERVICE PROPOSAL

TO,

CYRIX HEALTH CARE PVT .LTD

(Barcode: 0430507 – Ticket ID: 123843)

Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST	TOTAL PRICE IN INR
1	1KVA 24VDC INVERTER PCB	1	2200.00	2200.00	18	2596.00
2	12V 7Ah BATTERY	2	850.00	1700.00	28	2176.00
PAYABLE AMOUNT						4772.00

Commercial terms and conditions

1. Payment 80% advance along with PO balance before dispatch, 20% after installation.
2. Delivery period; 2weeks.
3. Tax :GST@18% for spares,28%@Battery
4. Installation; Our scope.

Please arrange to release the PO at our above address

Bank name :HDFC

Account no:50200082743176

IFSC Code:HDFC0004083

We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query.

Thank you,

Sincerely,

BHAGYAN

