



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 232718

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>SNCU in SAT Hospital</u></p> <p>Address <u>Thiruvananthapuram</u></p> <p><u>Kuala</u></p> <p>Ph : <u>9562317012</u></p>	<p>Call Registration Date : <u>10/7/24</u></p> <p>Caller ID : <u>122336</u></p> <p>Date of Visit : <u>6/8/24</u></p> <p>Asset No. : <u>0112643</u></p> <p>EQPT Name : <u>Oto Acoustic Emission Screener</u> <u>(OAE)</u></p> <p>Manufacture <u>Titan</u> Model : <u>NA</u></p> <p>S. No. <u>NA</u> Dept. <u>SNCU</u></p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working.

Action Taken : Checked and found that Motherboard and Clinical extension cable are damaged. Need to replace these spares for further checking and working condition of the equipment.


Completed Date : 6/8/24 Time : 6:20 PM Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Sreya Sudheep</u>	<u>6/8/24</u>	<u>6:00 PM</u>	<u>6:20 PM</u>

Customer Remark Completed Pending

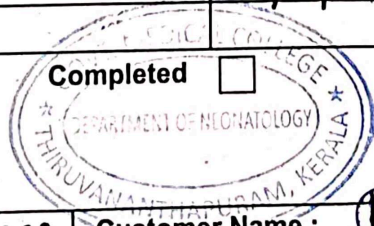

<p>Service Engineer Name : <u>Sreya Sudheep</u></p> <p>Signature : <u>Sreya</u></p> <p>Date : <u>6/8/24</u></p> <p>Contact Number : <u>7907406244</u></p>	<p>Customer Name : <u>Panagthy . eu .</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>6/8/24</u></p> <p>Contact Number : <u>984639993</u></p> <p>Designation : <u>Associate Professor</u></p> <p>Hospital Seal : <u>Head of The Department of Neonatology</u> <u>Govt Medical College Thiruvananthapuram</u></p>
---	---


577

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	SNCU IN SAT HOSPITAL
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : OAE MACHINE Make : Interacoustics Model : TITAN Serial No : SN8105122
4	Equipment ID/ Barcode	122336/0112643
5	Date of purchase/ Year of manufacture/Installation Date	17/03/2014
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	10/07/2024 (Toll free)
9	Action taken	Checked and found Motherboard and clinical extension cable defective. Need to replace these spares for further checking and working condition of the equipment. Enquired spares from vendor.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	Motherboard - 177000/- Clinical extension cable - 84370/- Total - 2,61,370/-

13	Asset Value	293328/-
14	* Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	89.1%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT AND ATTACHED
16	Reasons for recommending the equipments as BER	Checked and found Motherboard and clinical extension cable defective. The equipment was installed on 17/03/2014 and outlived up to 10+ years. The repairing cost is 89.1%. As per the tender clause 5.3.14.1 both criteria met. So recommending the unit for condemnation.
17	Name & Signature of CYRIX Authority	KASYEP P V 


*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Estimate for Mother board and clinical extension cable ~~defective~~ verified. Since the cost is high, it can be RBER as per guidelines.



7.08.2024

Signature of JC BM (NHM)


MANEESHA MOHAN M.R.

Junior Consultant (Biomedical)


National Health Mission

Thiruvananthapuram

Date:


Dr. RADHIKA.S
MBBS, DNB (Paed), DNB (Neonatology)
Associate Professor

Head of The Department of Neonatology
Govt. Medical College Thiruvananthapuram
Reg: No-28058

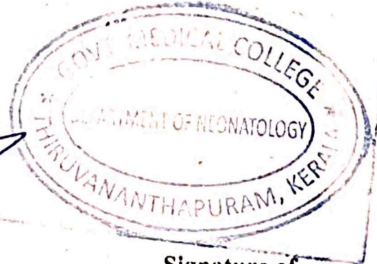

Signature of
Superintendent/Medical Officer (I/c)



V K HEALTHCARE SYSTEM

SHOP NO-01, GROUND FLOOR, KRISHNA COMPLEX,
 NEAR PNB BANK, KUND ROAD
 BEHROR Rajasthan 301701
 India
 Phone 7678531115
 Email- vkhealthcaresystem@gmail.com
 Website-www.vkhealthcaresystem.com
 GSTIN 08AZFPV9472M1ZB

Quotation

# Estimate Date	: VK/EST/24-25/75 : 20/07/2024	Place Of Supply	: Kerala (32)
-----------------	-----------------------------------	-----------------	---------------

Bill To	Ship To
CYRIX Healthcare Private Limited (Kerala) 1st Floor,30/641B Kochi Dhanushkodi Road Ernakulam 682038 Kerala India GSTIN 32AAFCC2499H2ZM	1st Floor,30/641B Kochi Dhanushkodi Road Ernakulam 682038 Kerala India

Subject :
 Regarding Titan OAE Sr Num- SN8105122

#	Item & Description	HSN/SAC	Qty	Rate	IGST		Amount
					%	Amt	
1	CLINICAL EXTENSION CABLE	90330000	1.00	71,500.00	18%	12,870.00	71,500.00
2	Motherboard	9033	1.00	1,50,000.00	18%	27,000.00	1,50,000.00

Total In Words
 Indian Rupee Two Lakh Sixty-One Thousand Three Hundred Seventy Only

Sub Total 2,21,500.00
 IGST18 (18%) 39,870.00
 Total ₹2,61,370.00

Notes

Looking forward for your business.

Company's Bank Details: V K Healthcare System
 Bank Name: HDFC
 A/C No: 50200080292598
 IFSC and Branch: HDFC0001839, Behror

Terms & Conditions

- Prices are FOR Destination.
- GST @ Extra. In case of any changes in the tax structure/ levies, the same shall be applicable at the time of invoicing and shall be borne by you.
- Delivery : 4 weeks from the date of receipt of your commercially and technically clear order.
- Payment : 100% advance by Demand Draft/Cheque/NEFT/RTGS.
- Other Taxes/Duties/Levies: Any local taxes or duties that are not applicable now but become leviable from the date of supply/bill shall be charged extra as applicable.
- Subject to Behror jurisdiction.
- Offer is subject to Force Majeure Clause.
- For Calibration- Need to send complete equipment through courier at our Head office.
- For Calibration- We need approximate 7 day in our office for complete process.



Authorized Signature



DR. RADHIKA.S
 MBBS, DNB (Paed), DNB (Neonatology)
 Associate Professor
 Head of The Department of Neonatology
 Govt. Medical College Thiruvananthapuram
 Reg:No-28058



Fw: Estimate - VK/EST/24-25/75 is awaiting your approval

1 message

Afsal Yunuze <zm1.klbemp@cyrix.in>
To: Kasyep P V <kasyepcyrix@gmail.com>

Fri, 26 Jul 2024 at 5:07 pm

QUOTATION FOR SAT OEA MACHINE

Regards

AFSAL YUNUZE

Zonal Manager (South Region)- Kerala

CYRIX HEALTHCARE Pvt. Ltd

30/641B, Petta, Poonithura, Kochi-38

Ph:+919895061437

From: V K Healthcare System <message-service@sender.zohobooks.com>

Sent: Thursday, July 25, 2024 5:07 PM

To: Afsal Yunuze <zm1.klbemp@cyrix.in>

Cc: ranakaran581@gmail.com <ranakaran581@gmail.com>; ranavikash87@gmail.com <ranavikash87@gmail.com>

Subject: Estimate - VK/EST/24-25/75 is awaiting your approval



Estimate #VK/EST/24-25/75

Dear CYRIX Healthcare Private Limited (Kerala),

Thank you for contacting us. Your estimate can be viewed, printed and downloaded as PDF from the link below.

ESTIMATE AMOUNT

₹2,61,370.00

Estimate No **VK/EST/24-25/75**

Estimate Date **20/07/2024**

VIEW ESTIMATE

Regards,

Vikash Rana

V K HEALTHCARE SYSTEM

