


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

Sl. No	Particulars	Details
1	Name of District	PALAKKAD
2	Name of Hospital	DISTRICT TB CENTRE
3	Name of Equipment with Make, Model and Serial Number	BIOCHEMISTRY ANALYZER MAKE : ROBONIK MODEL : PRIETEST TOUCH SN : AT0500412RBK
4	Equipment ID/ Barcode	0911853 # 124923
5	Date of purchase/ Year of manufacture/Installation Date	Ticket master installation date = Nil (As per stock book equipment installed on 30/07/2012 stock book attached for reference)
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	23/07/2024 (toll free)
9	Action taken	Checked the machine found not switching on. Problem with main Board and Display . Requested oem for quotation.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	RS.64760/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached OEM EOL letter attached
16	Reasons for recommending the equipment as BER	Checked the machine found not switching on. Problem main board and display. Requested oem for quotation. As per stock book equipment installed on 30/07/2012. aged up to 11 years 9 months. OEM informed that this model is obsolete. End of life letter issued As per tender clause 5.3.14.2 we recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AKHILESH P 


\*Not mandatory

#Based on the period of life and value as per the BER guidelines

\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Semiacuto analyser installed on 30/7/2012, aged up to 11 years. OEM submitted End of life certificate of this model. Hence recommended for RBER.

  
Signature of JC Bhat, Biomedical Consultant (NHM), Palakkad  
NHM (Arogyakeralam), Palakkad

Date:



  
7/8/20  
Signature of  
District Superintendent (Medical Officer) (i/c)  
District Hospital Compound,  
Palakkad, Pin-673 001



# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

**No. :** 231892

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>District TB Centre</u></p> <p>Address <u>Palakkad</u> <u>Kerala</u></p> <p>Ph : <u>8304090659</u></p>	<p>Call Registration Date : <u>23.07.2024</u></p> <p>Caller ID : <u>124923</u></p> <p>Date of Visit : <u>25.07.2024</u></p> <p>Asset No. : <u>0911853</u></p> <p>EQPT Name : <u>Semi Auto Biochemistry Analyser</u></p> <p>Manufacture <u>Robonik</u> Model : <u>Prietest touch</u></p> <p>S. No. <u>ATA500412R81</u> Dept. <u>Laboratory</u></p>
---	---

**Service Classification : Breakdown Call**  **PMS**  **Calibration**  **Cust.Training**

**Problem Identified :** Not working.

**Action Taken :** checked the equipment and found that machine not switching on. Problem with main board and display. Need to replace main board and display for further checking.

Completed  Date : 25.7.24 Time : 11:00 AM Spare Required

Spare Replaced  Requested

Sl. No.	Description	Qty.	Part Number	PR Number
1.	<u>nil</u>			
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Dileep. A.D</u>	<u>25.7.24</u>	<u>9:00 AM</u>	<u>11:00 AM</u>

**Customer Remark** Completed  Pending

**Service Engineer Name :** Dileep. A.D  
**Signature :** [Signature]  
**Date :** 25.07.2024  
**Contact Number :** 9048751999

**Customer Name :**  
**Signature :** [Signature]  
**Date :** 25.07.24  
**Contact Number :**  
**Designation :** District T. B. Officer,  
 District T. B. Centre,  
**Hospital Seal :** District Hospital Compound,  
 Palakkad, Pin-686 001



Date : 26.07.2024

Dear Valued Customer,



Thank you for choosing **Robonik (India) Pvt. Ltd.** We appreciate the opportunity to support our business. This letter is to inform you regarding the EOL (End of Life) of the instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT0500412RBK.**

As required, we stated herewith that the said instrument Semi Automated Biochemistry Analyser (Model : Prietest Touch) having **Serial No. AT0500412RBK** as **End of Life (EOL) Notified.** (During from installation is 10 years).

Thank you in advance for your understanding and your cooperation. If you have any questions, please contact our Customer Care Department at Toll Free No. 18005727977.

Yours faithfully,

For **ROBONIK (INDIA) PVT. LTD.**



Authorised Signatory




+91 98336 96980




+91 98336 96980  
 So you will make one List of instrument  
 send it to me

Ok 9:19 am ✓✓

26 July 2024

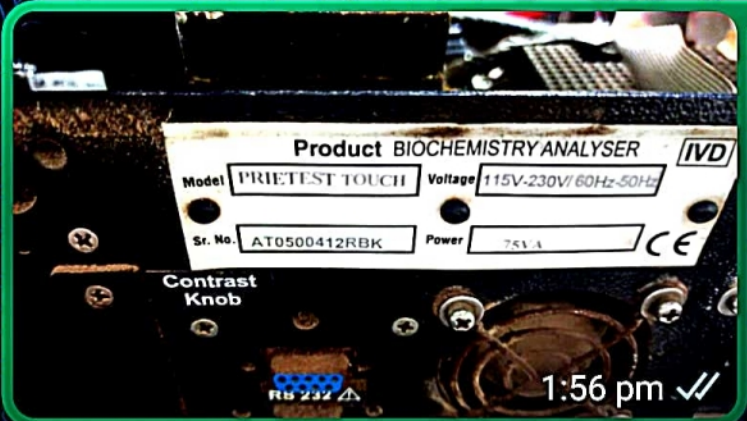

Forwarded

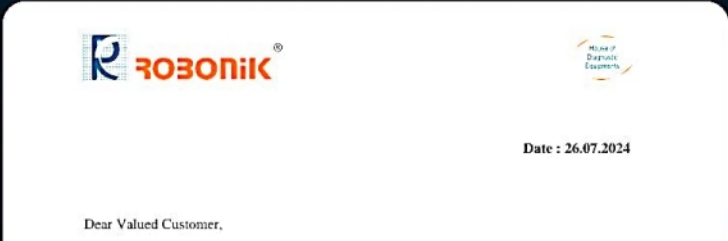

Dear Valued Customer,

EOL Letter = Prietest Touch -  
 AT0500412RBK.pdf  
 1 page • 89 kB • PDF

3:21 pm

Found 9 contact cards for this number. Add to your contacts?



Message    


SEMI AUTO ANALYSER.

				IN HAND STOCK balance	
30.7.12	FROM DTC STORE PKD WORTH Rs 84958/- (MAIN STOCK TBC REGISTER PAGE NO: 53)	1.000	1.000	1	6
	<u>ACCESSORIES</u>				
1	SINE WAVE UPS - 1.00				
2	HALOGEN LAMPS - 1.00				
3	THERMAL PRINT PAPER - 2.00				
4	DUST COVER - 1.00				
5	VARIABLE VOLUME PIPPET (10-100ul) 1.00				
6	FIXED VOLUME PIPPET. 500ul. 1.00				
	Issued to lab.				
	<u>REAGENTS</u>				
1	UREA MOD - 500ml				
2	CREATININE - 500ml.				
3	BILIRUBIN TEND. 500ml				
4	GLUCOSE 500ml				
5	CHOLESTRAL 500ml.				
6	QC. ABNORMAL 05ml				
7	QC NORMAL 05ml.				
30.7.2012	used in lab				1 NOS



*[Signature]*  
 District T. B. Officer,  
 District T. B. Centre,  
 District Hospital Compound,  
 Palakkad, Pin-673 002

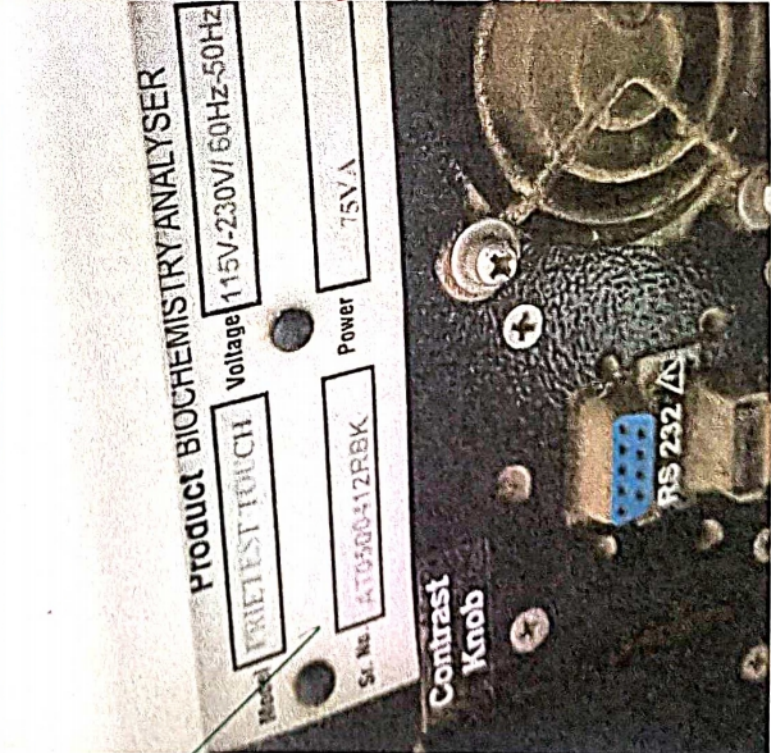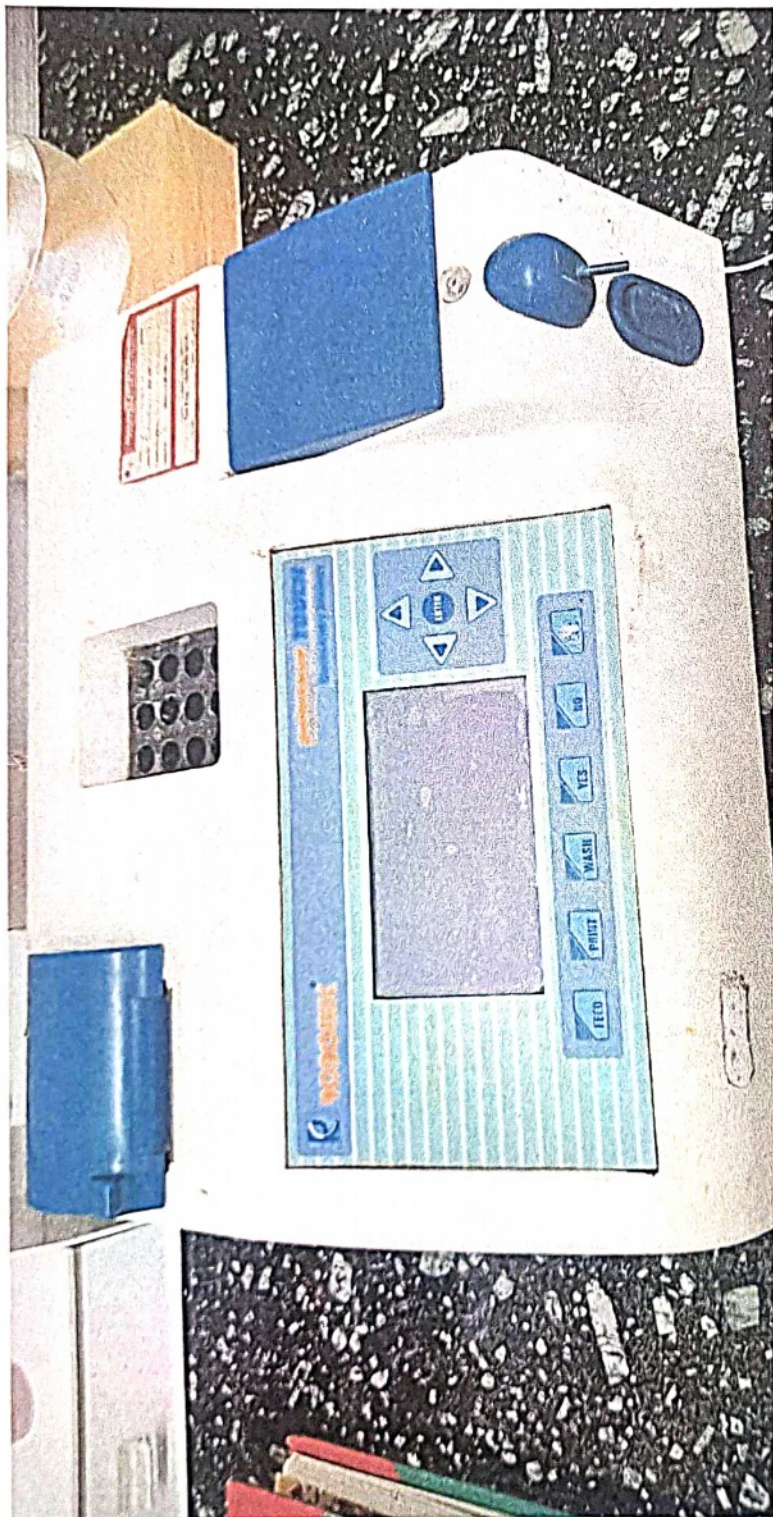

  
 District T. B. Officer,  
 District T. B. Centre,  
 District Hospital Compound,  
 Palakkad, Pin-673 004

0911853

Preventive Maintenance Schedule Kopl  
 01023/15/19  
 Q2

**CYRIX**  
 HEALTHCARE SYSTEMS  
 S.N: 01023/15/19  
 : 0911853  
 : 1879 723  
 : 1719 124  
 190 9001 - 2003, Certified Co. Ph: 374455972

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)  
 TOLL FREE NO: 1800 - 425-7669  
 BAR CODE - (8004-890615225)  
 0911853

**PRODUCT BIOCHEMISTRY ANALYSER**  
 Model: TRIEST TOUCH  
 Voltage: 115V-230V/ 60Hz-50Hz  
 Power: 75VA  
 S.I. No: 4T0300412RBK

