


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THRISSUR
2	Name of Hospital	GH Thrissur
3	Name of Equipment with Make, Model and Serial Number	Fully automatic biochemistry analyser Make - Erba Model - EM 360 S/N - 60242
4	Equipment ID/ Barcode	0810849 # 85820
5	Date of purchase/ Year of manufacture/Installation Date	Ticket master installation date 26-08-2011, As per stock book actual installation date is 18/10/2011
6	Warranty details	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown/ Date of registration of complaint	15/12/2023
9	Action taken	Checked the equipment and found RGT cooling assy with 6mm plate & spacer xlv2, assembly of photometer with packing, total internal tubing kit with connector, RIPT assy for XL-600. Big knf pump assy, cuvette ring set assembly and cuvettes are defective. Need to replace these spares for further service. Enquired for quotation from OEM.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Details of service required (Recommendations for repair)	Not recommending
12	Cost of spares (specify parts and cost)	RGT cooling aasy6mm plate & spacer klv2 -95335 Assembly of photometer with packing - 324875 /- Total internal tubing kit with connector- 75670/- RIPT assy for XL 600 – 72450/- Big Knf pump assy – 52210/- Cuvette ring set assembly – 49795/- Cuvettes - 49795/- GST – 179034.3/- TOTAL - 1173669 /-

13	Asset Value	10,82,525/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	108.44%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX.	Cyrix Service report, Quotation from OEM attached
16	Reasons for recommending the equipment as BER	Checked the equipment and found RGT cooling assy with 6mm plate & spacer xlv2, assembly of photometer with packing, total internal tubing kit with connector, RIPT assy for XL-600. Big knf pump assy, cuvette ring set assembly and cuvettes are defective. Enquired for quote from OEM. In Ticket master installation date is 26-08-2011 As per the stock book Equipment installed on 18/10/2011 and aged up to 12 years and 1 month. Spare cost is 108.44%, Both criteria met for RBER and as per Tender clause 5.3.14.1 We recommend this equipment for condemnation.
17	Signature of CYRIX Authority	BIJO T JOY 


*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Total spare cost is Rs 1173669/-
and almost twelve year finished


Signature of JC BM (NHM)


Consultant (Biomedical)
NHM, Thrissur

Date


GENERAL HOSPITAL
THRISSUR - PIN: 680 001


Signature of
Superintendent (Dy. DHS)
Superintendent/Medical Officer (i/c)
THRISSUR - PIN: 680 001



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 214135

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

Health Facility : <u>GH</u>	Call Registration Date : <u>15/12/2023</u>
Address : <u>THRISSUR</u>	Caller ID : <u>85820</u>
<u>KERALA</u>	Date of Visit : <u>16/12/2023</u>
Ph : <u>0487 2427383</u>	Asset No. : <u>0810849</u>
	EQPT Name : <u>fully automatic biochemistry analyser</u>
	Manufacture <u>Erba</u> Model : <u>EM-360</u>
	S. No. <u>60242</u> Dept. <u>Lab</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : check the equipment and found Double head vacuum pump, Urating assay, internal tubings, R. Arm assay, KWF pump Big, cuvette ring set, Cuvettes, stirrer assay are defective Enquired for quotation from OEM.

Completed Date : 16/12/23 Time : 2:30 pm Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>ABSIL TONY</u>	<u>16/12/23</u>	<u>1:30pm</u>	<u>2:30pm</u>

Customer Remark Completed Pending

Service Engineer Name : <u>ABSIL TONY</u>	Customer Name : <u>NISHA. KR</u>
Signature : <u>[Signature]</u>	Signature : <u>NISHAN</u>
Date : <u>16/12/2023</u>	Date : _____
Contact Number : <u>9745328470</u>	Contact Number : <u>9645283366</u>
	Designation : <u>LAB DEL</u>
	Hospital Seal : <u>SUPERINTENDENT (D.S)</u>



SUPERINTENDENT (D.S)
GENERAL HOSPITAL
THRISSUR - PIN: 680 001

QUOTATION

Bill To: CYRIX HEALTHCARE PVT LTD
First Floor,petta Junction 30/641b, Poonithura,Ernakulam, Kerala,
Pincode 682038 , Thrissur , Kerala 680001

Ref. No : 2425QUOTE001640
Date : Aug 7, 2024 11:30 AM
Validity : 30 days
TBM GSTIN : 27AAACTP2038C1ZT

Customer GSTIN No : 32AAFCC2499H2ZM

Ship to, District Hospital,Thrissur
G6C7+XJ3, Chembottil Ln, near Rangam Theatre, Kuruppam, Round
South , , Thrissur , Kerala 680001

SUB : QUOTATION FOR SUPPLY/REPLACEMENT OF SPARES IN INSTRUMENT MODEL: EM360 SR.NO.: 60242

With reference to the above, following Spares / Consumables are required to be replaced / supplied. Price/s of the same is / are given below, for approval:

SR. NO	Part Code	HSN Code	Description of Spares/Consumables	Qty	Unit Price	Discount%	GST%	Amount
1	114595	90278990	RGT COOLING ASSY WITH 6MM PLATE & SPACER_XLV2	1	95335		18	95335
2	103093	90278990	ASSEMBLY OF PHOTOMETER WITH PACKING	1	324875		18	324875
3	104951	90278990	TOTAL INTERNAL TUBING KIT WITH CONNECTOR (XL600/300/V2/A4/EM360)	1	75670		18	75670
4	105281	90278990	R1PT ASSY(SPARE) FOR XL-600/300-	1	72450	0	18	72450
5	182496	90278990	Big Knf Pump Assy.	1	52210	0	18	52210
6	182530	90278990	Cuvette Ring Set Assembly (WØ Cuvettes)	1	49795	0	18	49795
7	100279	70171000	CUVETTES	60	5405		18	324300
Merchant Name :TRANSASIA BIO-MEDICALS LTD						Total (Rs)		994635
SCAN AND PAY WITH UPI QR Merchant Name : TRANSASIA BIO MEDICALS LTD  Payee VPA : transasiabiomedicalsltd@citibank						Discount (Rs.) (-)		0
						GST (Rs.)		179034.3
						Rupees in words: Eleven lakhs Seventy Three thousand Six hundred Sixty Nine rupees and Three paise only		Grand Total (Rs.)

TERMS AND CONDITIONS :

- Payment :** Full payment should be made in advance through NEFT / RTGS/ Demand Draft in favour of "**Transasia Bio-Medicals Ltd**" to **Bank A/C no. : 00600330002538 IFSC code: HDFC0000060, UPI ID : transasiabiomedicalsltd@citibank.** You can also pay us through **UPI apps like BHIM/ Google Pay/ Paytm/PhonePe** etc. by scanning the above mentioned code. Cash Payment is strictly prohibited. No employee of the TBM is authorized to collect cash and or issue receipt against collection of Cash.
- GST :** As applicable
- Other Cost / Local duties :** Customer's responsibility
- Delivery :** Within 1-2 weeks from the receipt of your work order with payment confirmation

Thanking You
Your faithfully,
For **TRANSASIA BIO-MEDICALS LTD**

RECEIVED & ACCEPTED
CUSTOMER SIGNATURE & STAMP:
CUSTOMER NAME: _____
CONTACT NO: _____

TRANSASIA BIO-MEDICALS LTD.

Head Office: Transasia House. 8. Chandivali Studio Road, Andheri (E), Mumbai - 400 072. Tel.: (022) 4030 9000 Fax: (022) 2857 3030 Mumbai : Toll Free No. 1800 103 8226,
Whatsapp No.: 8451048434, SMS No.: 9212433444

www.transasia.co.in

DOC NO : SC00-405 / ISS - 7





REQUIRED QUOTATION FOR FULLY AUTOBIOCHEMISTRY ANALYZER 0810849 # 85820 @ GH TRISSURE , TRISSURE

3 messages

Akhilesh P <akhileshcyrix@gmail.com>
To: SANDEEP DAS M <s.das@transasia.co.in>


Mon, 29 Jul, 2024 at 11:38 am

Thanks & Regards

AKHILESH P
DISTRICT INCHARGE - PALAKKAD
Bemp-Kerala
Mobile : +91 7593847154
Email : akhileshcyrix@gmail.com

CYRIX HEALTHCARE (P) LTD
30/641B, Petta, Punithura
Ernakulam- 682038
www.cyrixhealthcare.com

On Sat, 27 Jul, 2024, 4:05 pm Mail Delivery Subsystem, <mailer-daemon@googlemail.com> wrote:



Address not found

Your message wasn't delivered to **s.das@transasia.o.in** because the domain transasia.o.in couldn't be found. Check for typos or unnecessary spaces and try again.

[LEARN MORE](#)

The response was:

DNS Error: DNS type 'mx' lookup of transasia.o.in responded with code NXDOMAIN Domain name not found: transasia.o.in For more information, go to <https://support.google.com/mail/?p=BadRcptDomain>

----- Forwarded message -----

From: Akhilesh P <akhileshcyrix@gmail.com>
To: s.das@transasia.o.in
Cc: Blesson Jose <Zm2.klbemp@cyrix.in>, DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Bijo T Joy <bijocyrix@gmail.com>
Bcc:
Date: Sat, 27 Jul 2024 14:32:19 +0530
Subject: REQUIRED QUOTATION FOR FULLY AUTOBIOCHEMISTRY ANALYZER 0810849 # 85820 @ GH TRISSURE , TRISSURE
Dear sir
Please share the quotation for biochemistry analyser @ GH TRISSURE , TRISSURE.

Details are furnished below.

Hospital Name : GH THRISSUR

Equipment Name : BIOCHEMISTRY ANALYZER

Make : ERBA

Model : EM360

SN : 60242

Thanks & Regards

AKHILESH P
DISTRICT INCHARGE - PALAKKAD
Bemp-Kerala
Mobile : +91 7593847154
Email : akhileshcyrix@gmail.com

CYRIX HEALTHCARE (P) LTD
30/641B, Petta, Punithura
Ernakulam- 682038
www.cyrixhealthcare.com

Akhilesh P <akhileshcyrix@gmail.com>
To: SANDEEP DAS M <s.das@transasia.co.in>

Mon, 5 Aug, 2024 at 9:20 pm

Dear sir
Kindly update the status.

Thanks & Regards

AKHILESH P
DISTRICT INCHARGE - PALAKKAD
Bemp-Kerala
Mobile : +91 7593847154
Email : akhileshcyrix@gmail.com

CYRIX HEALTHCARE (P) LTD
30/641B, Petta, Punithura
Ernakulam- 682038
www.cyrixhealthcare.com

[Quoted text hidden]

SANDEEP DAS M <s.das@transasia.co.in>
To: Akhilesh P <akhileshcyrix@gmail.com>

Wed, 7 Aug, 2024 at 11:38 am



Dear Akhilesh,

Please find the attachment and do the needfull

Get [Outlook for Android](#)

From: Akhilesh P <akhileshcyrix@gmail.com>
Sent: Monday, July 29, 2024 11:38:28 AM
To: SANDEEP DAS M <s.das@transasia.co.in>
[Quoted text hidden]

[Quoted text hidden]

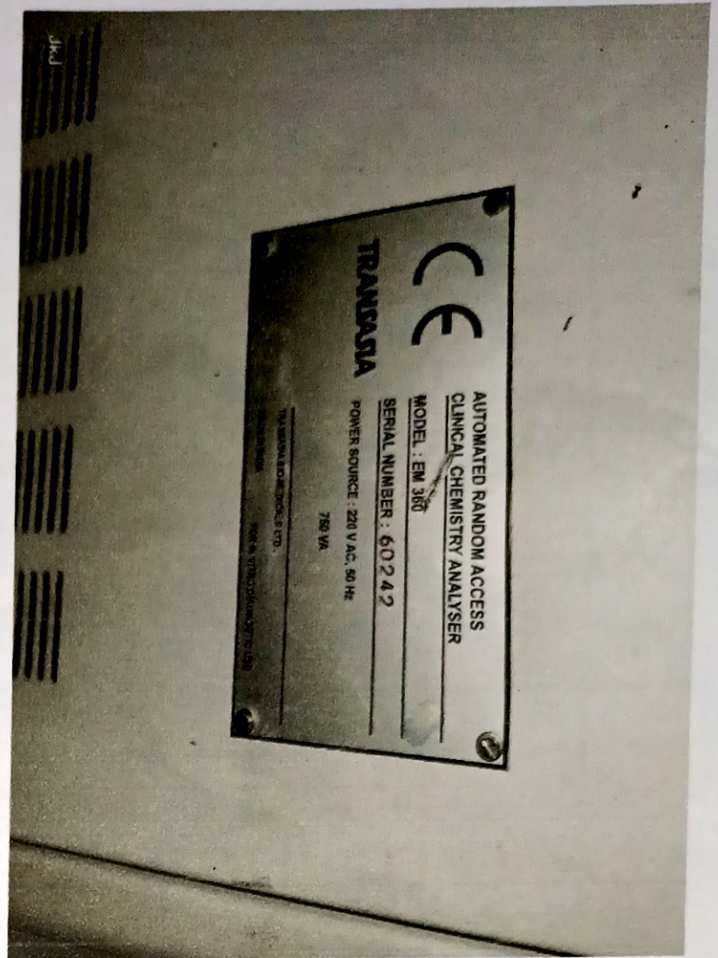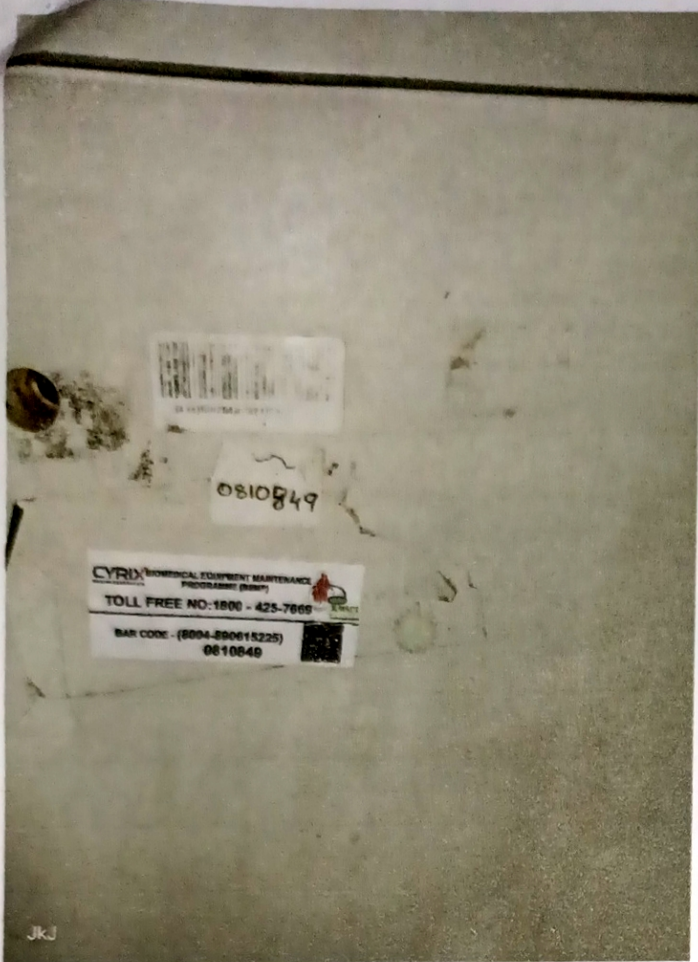

Handwritten signature in green ink.



**SUPERINTENDENT (Dy.DHS)
GENERAL HOSPITAL
THRISUR - PIN: 680 001**

STOCK BOOK OF INSTRUMENTS

Name of article Fully automatic random access clinical chemistry analyser. 183

Date	No. and Date of Invoice	From whom received or to whom issued	Receipt	Issue	Balance	Cost of article	Total No. on use	Initials of compliant authority
1	2	3	4	5	6	7	8	9
18/10/11	109 3440 19/3/11	Transasia bio medical Lab KMSCL order no: GMC (35/49) KMSCL/2010 dt. 10-2-11 <u>Accessories</u>	1		1	11,94,99.37	1	
		1. System Pack Demokit	1					
		2. Esba path (45 ml)	1					
		3. Water treatment plant	1					
		4. UPS	1					
		5. Refrigerator	1					
1/1/18		Mindway KMSCL order	1	1		1159345	2	
						1159345		
		<u>Accessories</u>						
		1. System pack Demokit	1					
		2. Esba 150 ml Plus	1					
		3. UPS on line 2 kv	1					
		4. Refrigerator 2/3 kw	1					
		5. UPS on line 2 kv	1					
		6. Computer	1					
		7. Control Panel	1					
		8. Refrigerator	1					
		9. Smoker	0000					
		10. mmsc 10-100 ml	5					
		11. mmsc 50 ml	5					
		12. Refrigerator	1					
		13. Billb H2O2						
		14. Delta line						
		15. Printer						



SUPERINTENDENT (Dy DMS)
GENERAL HOSPITAL
THRISSUR - PIN: 680 001