



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 216099

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>PHC ERATHU</u></p> <p>Address <u>ERATHU</u> <u>PATHANAMTHITTA</u></p> <p>Ph : <u>8921959814</u></p>	<p>Call Registration Date : <u>19/7/2024</u></p> <p>Caller ID : <u>124079</u></p> <p>Date of Visit : <u>22/7/2024</u></p> <p>Asset No. : <u>0340440</u></p> <p>EQPT Name : <u>B.P Apparatus</u></p> <p>Manufacture <u>Not available</u> Model : <u>BSX 515</u></p> <p>S. No. <u>515CB15</u> Dept. <u>Main Center</u></p>
-------------------------------------------------------------------------------------------------------------------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : checked and found that main board, display board, battery sockets, battery and accessories are defective

Completed Date : 22/7/24 Time : 12:00pm Spare Required

Spare Replaced Requested

No.	Description	Qty.	Part Number	PR Number
1.				
2.				
3.				

Cyrix Engineer	Date	Start Time	End Time
<u>Manish R Nain</u>	<u>22/7/24</u>	<u>10:00am</u>	<u>12:00pm</u>

Customer Remark Completed Pending




<p>Service Engineer Name : <u>Manish R Nain</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>22/7/24</u></p> <p>Contact Number : <u>9365109472</u></p>	<p>Customer Name : <u>[Signature]</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>22/7/24</u></p> <p>Contact Number : <u>[Blank]</u></p> <p>Designation : <u>Medical Officer, In-Charge</u></p> <p>Hospital Seal : <u>Primary Health Center Erathu</u></p>
----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER) PERFORMA

Sl. No	Particulars	Details
1	Name of District	PATHANAMTHITTA
2	Name of Hospital	PHC ERATHU
3	Name of Equipment with Make, Model and Serial Number	Name-B P Apparatus Make-Not available Model-BSX515 Sl.no- 515CBL15
4	Equipment ID & Barcode	124079 & 0340440
5	Date of purchase / Year of manufacture / Installation Date	11/02/2021
6	Warranty details (Yes/No)	Not Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	Not AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	19-07-2024
9	Action taken	Checked and found that Main board, display board, battery sockets, battery and accessories are defective.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully Damaged
11	Recommendations for repair (required service details)	Not recommended for repair
12	Cost of spares (specify parts and cost)	Not Available

13	Asset Value	Rs.1417/
14	#Percentage value of the cost of spareswith respect to Cost of Purchase/ Asset Value	Not Available
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service Report attached
16	Reasons for recommending theequipment as BER	Checked and found that Main board, display board, battery sockets, battery and accessories are defective. Quotation not submitted since spare parts are not available in market. So, equipment recommended for RBER.
17	Name & Signature of CYRIX Authority	MANISH R NAIR 


*Not mandatory

#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Physically verified on 06.08.2024. Inspected and found all parts are defective, items recommended to BER as per rule




12.8.24 Con BME

CONSULTANT(BIOMEDICAL)
NATIONAL HEALTH MISSION
PATHANAMTHITTA

Date

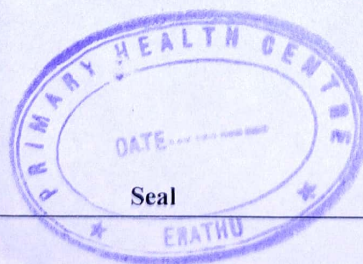


11/08/24

Signature of
Superintendent / Medical Officer (i/e)



Medical Officer, In - Charge
Primary Health Centre
Erathu

Date of Recpt	Cal. No Date	From	Items received or to whom issued	Receipt Num	Batch No
3/9/19	1295 2.9.2019	Rel forms Karunya Thiruvally	B/p forms the stock registered N/M page no: (49)	1	2
			Batch NO: 112 Exp. 12/2028	1	3
	1319 2.9.19		Batch no: 112	1	4
	1299 2.9.19		Batch no: 112	1	5
	1297 2.9.19		B. no: 112	1	6
			B. no: 112	1	5
4/9/19			This one issued to LHI for subcenter	5	5
23.4.20			Issued to SPN. (SPN Reg P no: 27)	01	NIC
			Incident sanctioned by <i>[Signature]</i>		
22.3.21	26066 22.3.21		Karunya Community pharmacy		
			B. no: 115 exp. dt: 12/28 Rate: 1265 Net Amount: 1417.0	01	01
22.3.21			Issued to palliative nurse. <i>[Signature]</i>	01	NIC
11.2.21			Karunya Community pharmacy		
11.2.21	23304 11.2.21		B. no: 115 exp. dt: 12/28 Rate: 1265 (Digital) Net Amount: 1417.0	01	01
11.2.21			Issued to staff nurse. <i>[Signature]</i>	01	NIC
			Incident sanctioned by <i>[Signature]</i>		
7/3/22	24528 7/3/22		Karunya Community pharmacy		
			B. no: 1115 exp. dt: 5/26 (Digital) Rate: 1265.0 cost 6%	02	02
7/3/22			Issued to HI	02	NIC
7/3/22			Issued to staff nurse. <i>[Signature]</i>	01	NIC
			Incident sanctioned by <i>[Signature]</i>		
2/2/22			Received from DCC (Digital)	01	01
28/3/22			Issued to RHI <i>[Signature]</i>	01	NIC
			Incident sanctioned by <i>[Signature]</i>		



[Signature]
Medical Officer, In-Charge
Primary Health Center
Erathil

do page no: (63)

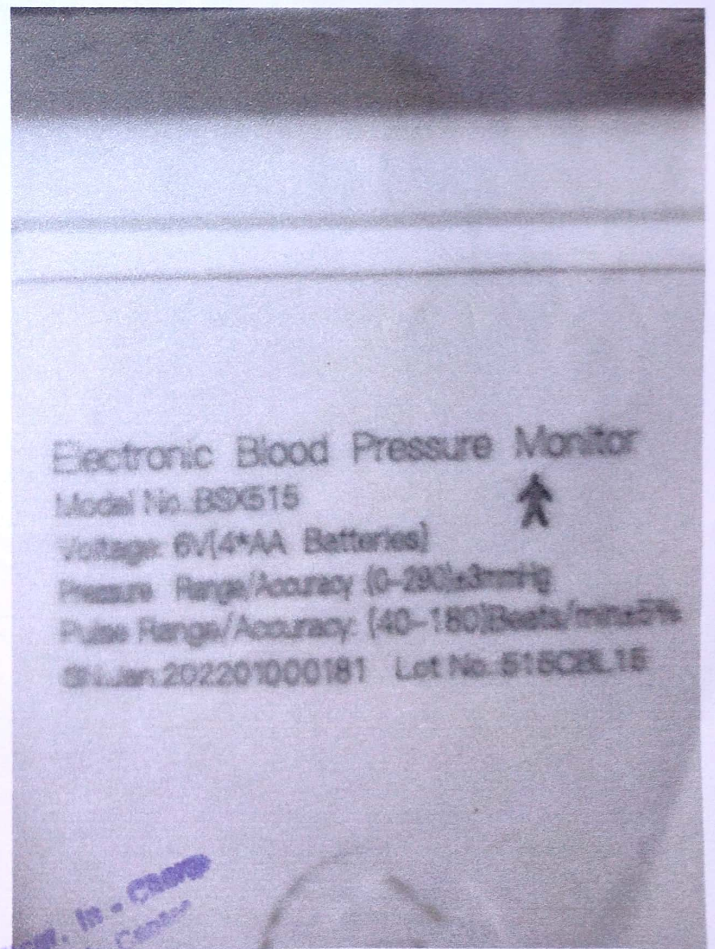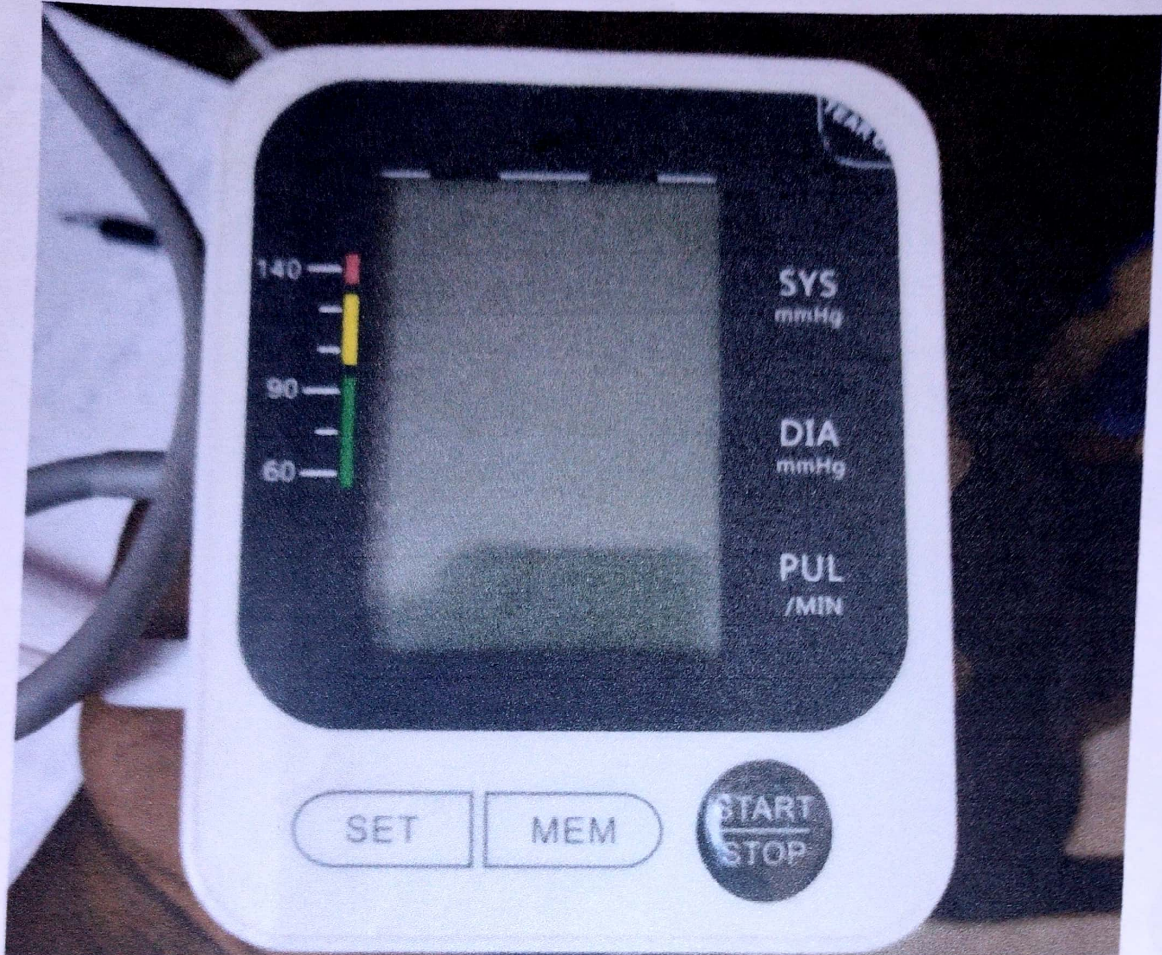

Subin
No. 22

Medical Officer, In-charge
Primary Health Center