



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :

229462

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>PHE Parathodu</u></p> <p>Address <u>Kottayam</u></p> <p>Ph : <u>8136803861</u></p>	<p>Call Registration Date : <u>11-07-24</u></p> <p>Caller ID : <u>122501</u></p> <p>Date of Visit : <u>13-07-24</u></p> <p>Asset No. : <u>0542963</u></p> <p>EQPT Name : <u>BP Apparatus</u></p> <p>Manufacture <u>HIL</u> Model : <u>HIL</u></p> <p>S. No. <u>HIL</u> Dept. <u>OP</u></p>
--	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : checked and found that NIBP pump and main PCB faulty. Need to replace these spares. Post further checking and working condition.

Completed Date : 13/7/24 Time : 10:00 Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Ajmal shajahan</u>	<u>13/7/24</u>	<u>10:00</u>	<u>12:00</u>

Customer Remark Completed Pending



Handwritten notes and signatures:
W
Dr. Umma K. Parathodu
13/7/24
Parathodu
District

Service Engineer Name : Ajmal shajahan
 Signature : [Signature]
 Date : 13/7/24
 Contact Number : 9491215618


Customer Name : Shennik Sebastian
 Signature : [Signature]
 Date : 13/7/24
 Contact Number : 7038980970
 Designation : JPHM
 Hospital Seal :

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KOTTAYAM
2	Name of Hospital	PHC PARATHODU
3	Name of Equipment with Make, Model and Serial Number	Equipment :Digital B P Apparatus Make :Nill Model :Nill SN:Nill
4	Equipment ID & Barcode	122501 & 0542963
5	Date of purchase / Year of manufacture /Installation Date	01/09/2021
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	11-07-2024 (Toll free)
9	Action taken	Checked and found out the problem with main PCB and Nibp pump
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	N/A

13	Asset Value	Rs .2350/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report attached
16	Reasons for recommending the equipment as BER	Checked and found out the problem with main PCB and NIBP pump. Machine installed in 01/09/2021 and covered up to ? 2+ years. Quotation not submitted since spare are not available in the market. So recommended the machine for condemnation
17	Name & Signature of CYRIX Authority	Ajmal shajahan 


*Not mandatory **#Based on the period of life and value as per the BER guidelines**


* **Attach Photograph**

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Asset value - 2350
 cost of spare - not submitted
 life period. - 2 year 11 months.
 As per the BER guidelines life period criteria satisfied only (1/9/2021) after 1/9/2024 -



 Signature of JC BM (NHM)
 CONSULTANT BIOMEDICAL ENGINEER
 NATIONAL HEALTH COMMISSION
 KOTTAYAM

Date 

FOR DR. UNNIKRISHNAN
 Dated: 18/7/23 DR TAJA 
 Signature of
 Superintendent / Medical Officer (i/c)
The Medical Officer in-charge
 F. H. C. Parathodu
 Kottayam District

BP APPARATUS - DIGITAL



- 01/09/2021 Received from CELTC Pochimattom
[CELTC Instruments Register
Page No: 10] Model No: EL-510 → 5 nos. 5 nos.
Date of Inposal: Nov. 2020 ^{Rate - 1800 + 12% GST} MRP - 2199/-
- 14/01/09/2021 Issued to JHI, DCC Jc → 1 no. 1 no. 5 nos.
Marketed by Nitko Surgicals
Product by Lifecare enterprises, MRP - 2350/-
m/s on July 20 (341-444)
J. Mathan
Jr. 1st m. 2
- 13/05/2022 Issued to Palliative Nurse → 1 no. 4 nos.
- 20/08/22 Issued to Nursing officer → 2 nos. 2 nos.
[S/N - Substock Reg. for Equipments & Instruments
Page No: - 76]
Shobana S.M
- 22/03/23 Issued to LHI → 1 no. Nil
[MLSP Stock Book
Page No: - 1]
A. S. Preethi S.

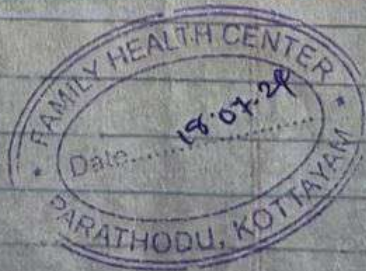

FOR DR. UNNIKRISHNA

DR. STANIA

The Medical Officer in Charge
F. H. C. Parathodu
Kottayam District

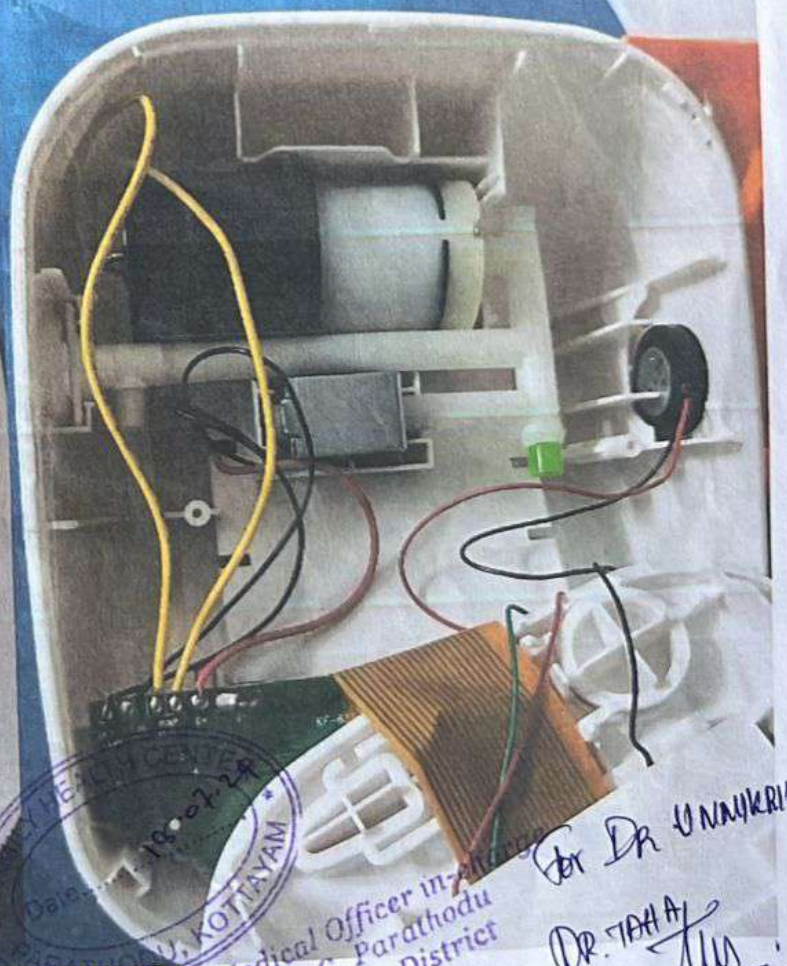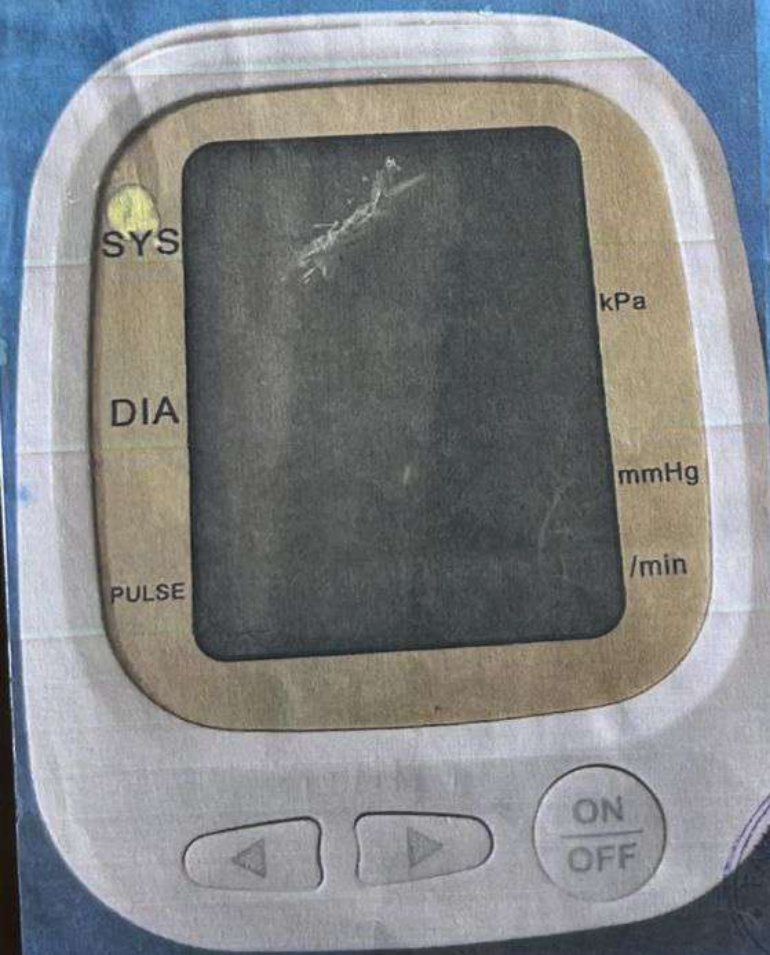

HEALTH CENTRE
PARATHODU, KOTTAYAM
Date: 18-07-24

The Medical Officer in-charge
F. H. C. Parathodu
Kottayam District

For Dr. V. N. KRISHNA
DR. TAHA
72469