



**BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAMME
UNDER
NATIONAL HEALTH MISSION**



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX
HEALTHCARE PVT LTD

No. : 232892

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Potta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrilx.com | E-mail : bomp.kl@cyrilx.in

Health Facility <u>Phe</u>	Call Registration Date : <u>08/07/24</u>
Address <u>Killimanoor</u>	Caller ID : <u>12704</u>
<u>Thiruvananthapuram</u>	Date of Visit : <u>10/07/24</u>
Ph : <u>8281733040</u>	Asset No. : <u>0145396</u>
	EQPT Name : <u>oxygen concentrator</u>
	Manufacture <u>yuwell</u> Model : <u>NA</u>
	S. No. <u>NA</u> Dept. <u>OP</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : Checked and found mainboard compressor and serve bed complaint need to replace these spare for further checking and working condition of the equipment. Enclosed spares from OEM


Completed Date : 10/7/24 Time : 11:45 Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrilx Engineer	Date	Start Time	End Time
<u>Deepak. E-M</u>	<u>10/7/24</u>	<u>11 am</u>	<u>11:45</u>

Customer Remark Completed Pending

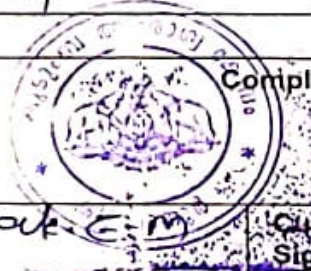

Handwritten notes in Malayalam script

Service Engineer Name : Deepak. E-M
Signature : [Signature]
Date : 10/7/24
Contact Number : 7902881038

Customer Name : Ray. S. Nav
Signature : [Signature]
Date : 10/7/24
Contact Number : 9842391393
Designation : [Signature]
Hospital Seal :

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	PHC KILIMANOOOR
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : Oxygen concentrator Make : Yuwell Model : NA SL : NA
4	Equipment ID/ Barcode	121704 /0145396
5	Date of purchase/ Year of manufacture/Installation Date	22/09/2021
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	08/07/2024(Toll free)
9	Action taken	Checked and found Mainboard, compressor and seive bed complaint. Need to replace these spare for further checking and working condition of the equipment. Enquired spares from OEM.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE


MEDICINE STOCK REGISTER


143


Name of article..... Oxygen Concentrator

From page No..... To page No.....

Date	Received	Issued	Balance	Remarks
30/11	From District Drug Warehouse (Covid Donations)			From District Drug Warehouse (Covid Donations)
5/12/21	Issued to S/N			
31/12/21	From No. 42001/ED/01069/21-22 dated 30.12.21			From District Drug Warehouse (Covid Donations)
5/1/22	Issued to S/N			
11/1/22	Hand Sanitizer Dispensing	2	2	
16/1/22	Issued to S/N			


 സി. കെ. ജോർജ്ജ്
 ഡി. ഡ്രഗ് ഹൗസ് ഓഫീസർ
 ഡി. ഡ്രഗ് ഹൗസ്
 കോട്ടയം

Received

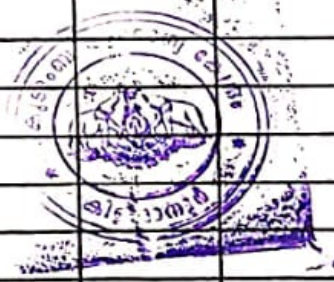 A1



**EQUIRY-QUOTATION-YUWELL-OXYGEN CONCENTRATOR-PHC
KILIMANOOR(0145396/121704)**

5 messages

Kasyep P V <kasyepcyrix@gmail.com>

Sat, Jul 13, 2024 at 11:22 PM

To: "sales@yuwell.co.in" <sales@yuwell.co.in>

Cc: Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>, Project Manager KLBEMP <pm.bempkl@cyrix.in>

Dear sir,

I'm reaching out to enquire about the spare quotation for the Oxygen concentrator. Make :

Yuwell

Model : 7F 10

Spares Quotation required for;

- 1.Mainboard
- 2.Compressor
- 3. Sieve Bed (2 nos)

--

Thanks & Regards,

KASYEP PV

District Incharge ,Trivandrum

CYRIX HEALTHCARE Pvt.Ltd

KLBEMP

Ph : +91 7593847134 kasyepcyrix@gmail.com

Kasyep P V <kasyepcyrix@gmail.com>

Mon, Jul 15, 2024 at 10:44 AM

To: sales@yuwell.co.in

Cc: Afsal Yunuze <zm1.klbemp@cyrix.in>, DM Abijith-KLBEMP <dm2.klbemp@cyrix.in>, Project Manager KLBEMP <pm.bempkl@cyrix.in>

Sir,

Consider this mail as a gentle Reminder

[Quoted text hidden]

[Quoted text hidden]

Kasyep P V <kasyepcyrix@gmail.com>

Sat, Aug 3, 2024 at 3:04 PM

To: Mahaveer Singh <sales@yuwell.co.in>

[Quoted text hidden]

Kasyep P V <kasyepcyrix@gmail.com>

Tue, Aug 6, 2024 at 12:59 AM




To: Mahaveer Singh <sales@yuwell.co.in>

Sir,

Gentle Reminder

[Quoted text hidden]



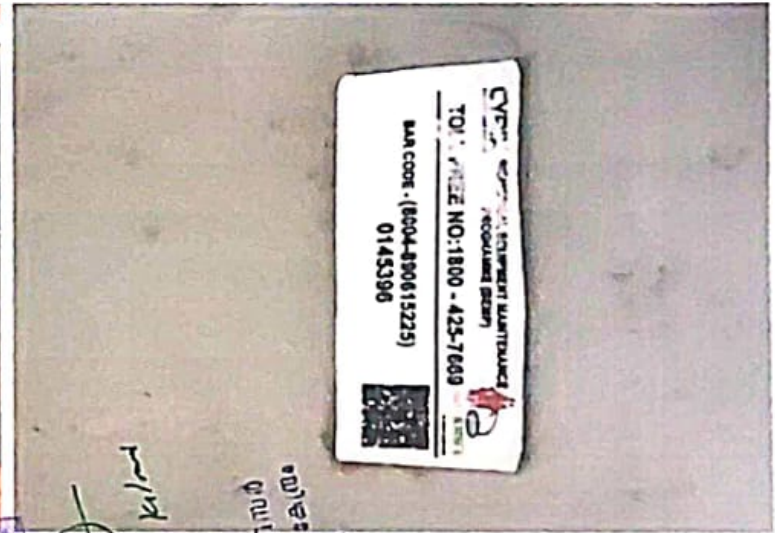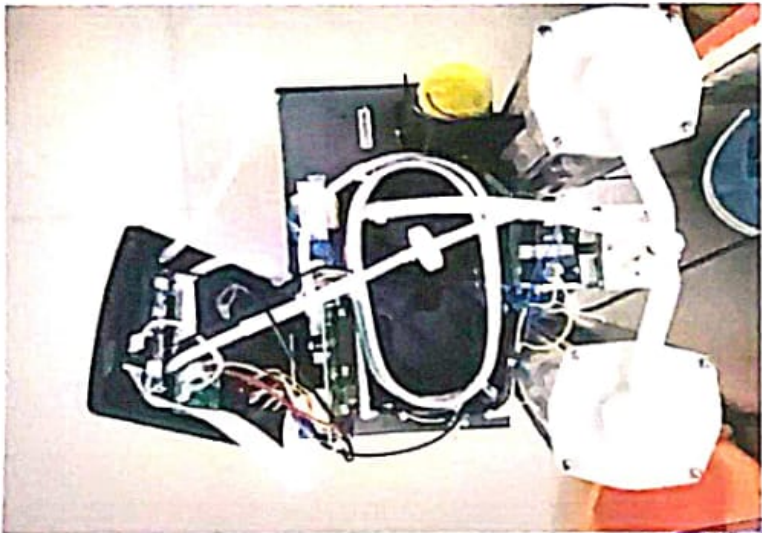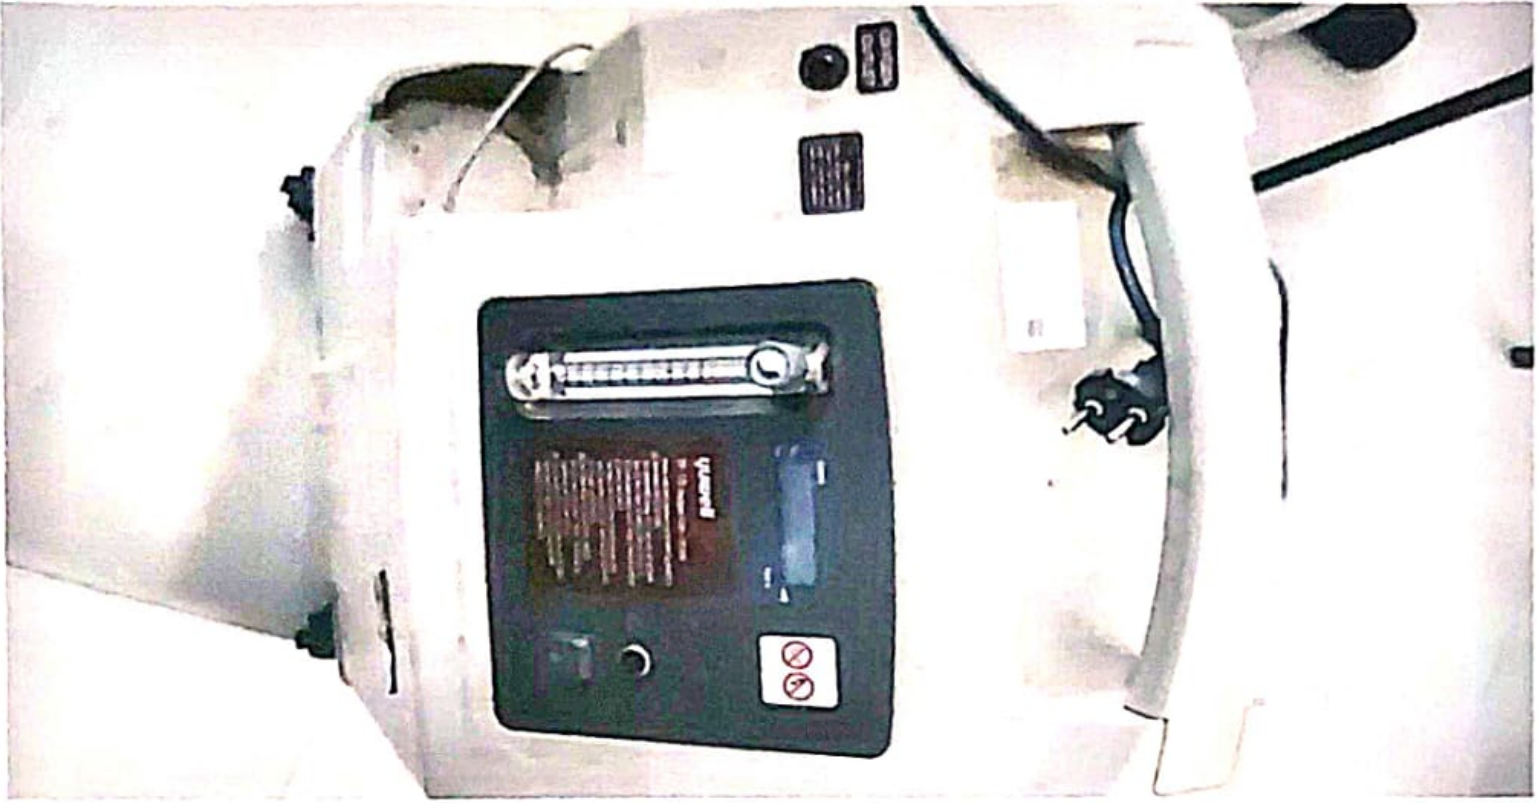

CVC EQUIPMENT MAINTENANCE
 (REGULATED BY THE)
TEL: PHONE NO: 1800 - 425-7609
SAM CODE: (8004-890615225)
01453396



Handwritten text in a non-Latin script, including a signature and several lines of notes.