



**BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAMME  
UNDER  
NATIONAL HEALTH MISSION**



SERVICE PROVIDER  
Tender No. WO-37/2021-2022/698

**CYRIX**  
HEALTHCARE PVT LTD

No. : 220255

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report**

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility : <u>GH Pala</u>	Call Registration Date : <u>4/7/2024</u>
Address : <u>Kottayam</u>	Caller ID : <u>121020</u>
Ph : <u>9605841191</u>	Date of Visit : <u>6/7/2024</u>
	Asset No. : <u>0511204</u>
	EQPT Name : <u>OT Light</u>
	Manufacture <u>Hospitech</u> Model : <u>Hospilite 1001</u>
	S. No. <u>Nil</u> Dept. <u>OT</u>

Service Classification : Breakdown Call  PMS  Calibration  Cust.Training

Problem Identified : Not working

Action Taken : checked the machine Bulb, Bulb holder, Transformer and Bulb reflector are fully damaged and handles/Arms fully rusted not working properly

Completed  Date : 6/7/2024 Time : 11am Spare Required

Spare Replaced  Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer

Josekutty George

Date

6/7/2024

Start Time

10am

End Time

11am

Customer Remark

Not Working

Completed

Pending

Service Engineer Name : Josekutty George

Signature : [Signature]

Date : 6/7/2024

Contact Number : 8848230407

Customer Name : Sreelakshmi K


Signature : [Signature]

Date : 6/7/2024

Contact Number : 9605841191

Designation : Srv.

Hospital Seal :




**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

Sl. No	Particulars	Details
1	Name of District	KOTTAYAM
2	Name of Hospital	GH PALA
3	Name of Equipment with Make, Model and Serial Number	Equipment :OT LIGHT Make: HOSPITECH Model :1007 SN:NIL
4	Equipment ID & Barcode	121020 & 0511204 ✓
5	Date of purchase / Year of manufacture /Installation Date	13/9/2005
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	04/07/2024 (Toll free) ✓
9	Action taken	Checked and found out the problem with transformer, lamp, lamp holder and handles arm need to be repaint because of rust in condition
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not recommending for repair.
12	Cost of spares (specify parts and cost)	N/A

13	Asset Value	Rs . 46000/-
14	#Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	N/A
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix service report are attached
16	Reasons for recommending the equipment as BER	Checked and found out the problem with transformer, lamp, lamp holder and handles arm need to be repaint because of rust in condition. Machine installed in 13/09/2005 and covered up to 18 + years. So recommending the machine for condemnation
17	Name & Signature of CYRIX Authority	Josekutty George 

\*Not mandatory #Based on the period of life and value as per the BER guidelines


\* **Attach Photograph**


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Asset value = 46,000  
 cost of spares = Not mentioned -  
 Life period - 18 years  
 Reasons for BER - transformer, Lamp, lamp holder and handles - damaged and rusted (as per service report)

  
 CONSULTANT BIOMEDICAL ENGINEER  
 NATIONAL HEALTH BUREAU  
 KOTTAYAM  
 Signature of J.C. BM (NHM)




Date

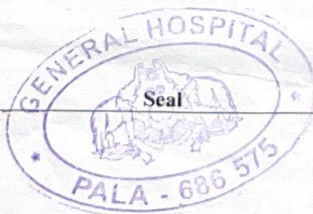

  
 26/7/24  
 Signature of  
 Superintendent / Medical Officer (i/c)

**SUPERINTENDENT**  
 Govt. General Hospital  
 Pala, Kottayam.

**LYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)**  
TOLL FREE NO: 1800 - 425-7669  
BAR CODE - (8004-890615225)  
0511204

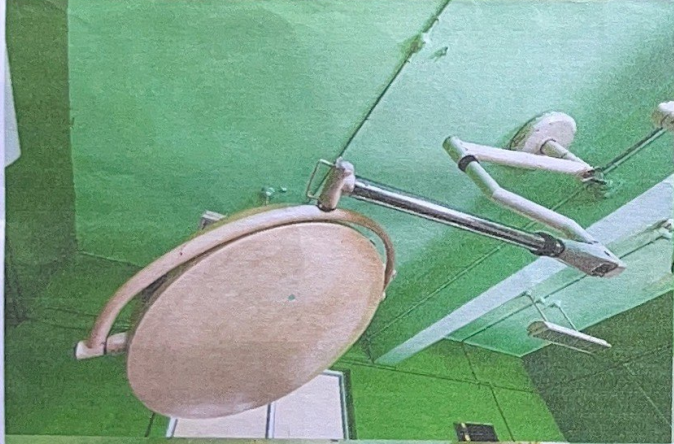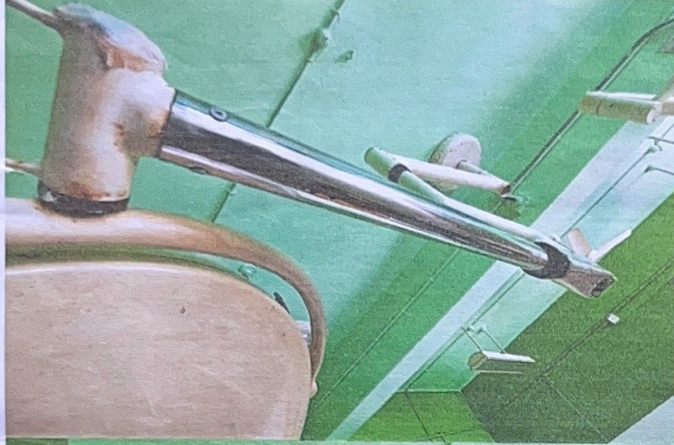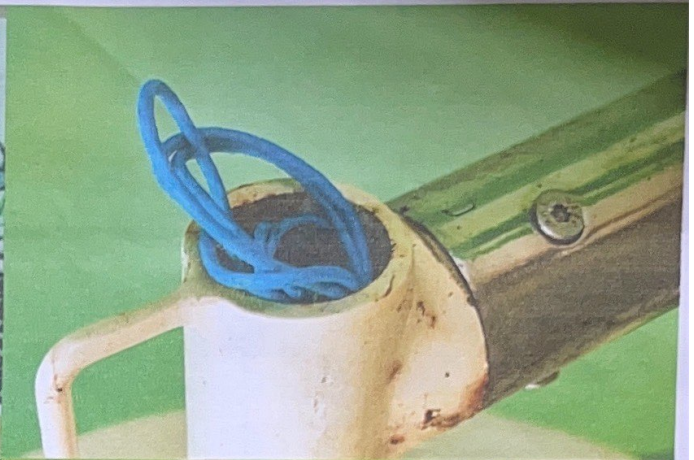


PORTABLE + ROOF MOUNTED

051

Model	Warranty	A.m.c	Issued to Dept	S.S Page no	Main No
Hospital 1007	-	-	Issued to OT	122	247/IV
-	-	-	Issued to OT	122	247/IV
-	-	-	Issued to OT	122	252/IV

~~PRINTED~~  
26/7/24

SUPERINTENDENT  
Gorla Sagar Hospital  
Peta, Kottayam

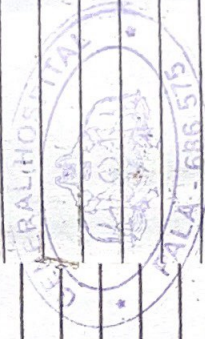

SHADOW LESS LAMP

050

dt of Rt dt of hospital	Qty	Warranty	Warranty (Roof mounted)	Net mch cost	Capacity	Name of mch	Diffs supply
10-9-05	1	✓	Warranty	46000/-			
3-2-06	1	✓	Warranty	75460/-	12.5%	L.P. Vol X	Page 57
3-2-06	1	✓	Warranty	Rs 16,836/-	12.5%	L.P. Vol X	Page 57 X