



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 227352

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility : <u>THQ#</u></p> <p>Address : <u>THQ# Karunayappally</u> <u>KOCCAM</u></p> <p>Ph : <u>9846987701</u></p>	<p>Call Registration Date : <u>7/06/24</u></p> <p>Caller ID : <u>115705</u></p> <p>Date of Visit : <u>8/06/24</u></p> <p>Asset No. : <u>0220458</u></p> <p>EQPT Name : <u>spot light</u></p> <p>Manufacture <u>Hardik meditech</u> Model : <u>Spax led Foot</u></p> <p>S. No. <u>SL/18-19/025</u> Dept. <u>OT</u></p>
--	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Light not getting on

Action Taken : Checked the spot light found that the
amps, control PCB, lens, wheel, adjustable spring
are defective need to replace these spares for
further checking and working condition of
equipment. To give spares with OEM.

Completed Date : 8/06/24 Time : 11:30 AM Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrux Engineer	Date	Start Time	End Time
<u>Diswanya Raj k N</u>	<u>8/06/24</u>	<u>10:45 AM</u>	<u>11:30 AM</u>

Customer Remark _____ **Completed** **Pending**

<p>Service Engineer Name : <u>Diswanya</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>8/06/24</u></p> <p>Contact Number : <u>9645384968</u></p>	<p>Customer Name : <u>Saleem</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>8/6/24</u></p> <p>Contact Number : <u>SND</u></p> <p>Designation : <u>SND</u></p> <p>Hospital Seal : <u>9846987701</u></p>
---	--

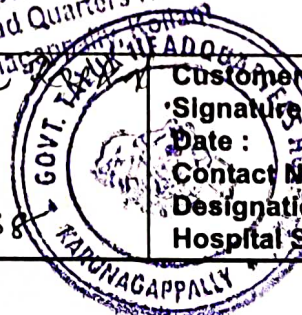


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	Kollam
2	Name of Hospital	THQH KARUNAGAPPALLY
3	Name of Equipment with Make, Model and Serial Number	SPOT LIGHT Make : HARDIK MEDITECH Model : SPARX LED F004 SI no: SL/18-19-025
4	Equipment ID & Barcode	Barcode : 0220458 / Ticket id : 115705
5	Date of purchase / Year of manufacture /Installation Date	25-06-2018
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No AMC/CAMC
8	Date of breakdown(Date of registration of complaint through email/ Toll free)	07-06-2024
9	Action taken	Checked the machine found that Smmps, control pcb, wheel, Adjustable spring, lens are defective, Enquired spares with OEM
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	Not Recommended for Repair
12	Cost of spares (specify parts and cost)	SMPS driver = 2950 Touch sensor with Control PCB = 3540 Led Projection Lens = 1770 Wheel 4 nos = 1416 Adjustable spring for arm = 2714 Total = 12390 /-


13	Asset Value	Rs. 16630 /-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	74.50 %
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report & OEM Quotation attached
16	Reasons for recommending the equipment as BER	Checked the machine found that the Smpls, control pcb, wheel, Adjustable spring, lens are defective. Equipment is installed on 07-06-2024 and aged up to 5years 11 month. .Repairing cost of equipment is 74.50%. as per tender clause 5.3.14.1 Both criteria met So we are recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	AISWARYA RAJ 

*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Repairing cost is high - So recommended for Beyond economic repair


 05.07.24
 Signature of A. B. M. (NHM)
 NHM, KOLLAM

Date



26
 Superintendent /
 Medical Officer (i/c)
 Superintendent
 Taluk Head Quarters Ho-
 Karunagappally, Kolla

BCS Healthcare Pvt.Ltd
3136,11nd door,Mathewsons square
MetroPillar No:464 NearChangapuzha park
Cochin, Kerala – 682024,
Email : Info@bcshealthcare.in
web: www.bcshealthcare.in



GST NO: 32AAKCB2766M1Z

DATE: 01/07/2024

Ref: BCS/89/24-25

QUOTATION

TO,

CYRIX HEALTHCARE PVT LTD

Subject: Quotation for Spot Light Service

SL.NO	PRODUCT NAME	QTY	UNIT RATE	TAX 18%	TOTAL
01	SMPS driver	1	2,500.00	450.00	2,950.00
02	Touch Sensor With Control PCB	1	3,000.00	540.00	3,540.00
03	Led Projection Lens	1	1,500.00	270.00	1,770.00
04	Wheel 4 Nos	1	1,200.00	216.00	1,416.00
05	Adjustable Spring For Arm	1	2,300.00	414.00	2,714.00
Grand Total					12,390.00

Terms & Conditions

- Delivery within 8 days after confirmation of purchase order
- Tax are included
- Payment 50% advance balance 50% after delivery time





Superintendent
Taluk Head Quarters Hospital
Karunagappally, Kollam

For, BCS HEALTH CARE PRIVATE LIMITED

SHADOW LESS LAMP + HALOGEN LAMP B1


Date	Name	Received	Issued	Balance	Remarks
27/2/12	Tr. in from old stock book Pg No. 48 Shadowless lamp Halogen lamp double dome ceiling mount (2nd) 16/6/15		Vol. I.		
12/12/2011	Rd from Stock PHILIPS Spot light (major light) cost 1, 29200. Page 164	1		1	
26/10/13	Rd from Stock Philips OT light - in stock Page - 165 - Rs - 65194 model - 59, mobile code no 91-45	1		2	
26/3/14	Rd from Stock cost - 50933 model - LMA 17A mobile - Spot light.	1		3	
16/6/15	Rd Halogen Lamp double dome ceiling mount model - 500-P Rs - 3,8000 m-s page no. 253 484 - 23 55558	2 set		5	
25/6/2014	Rd mobile spot light m-s (205) 20k cost 16,630 + 12% tax	1		6	Go

(Praveen Techno)

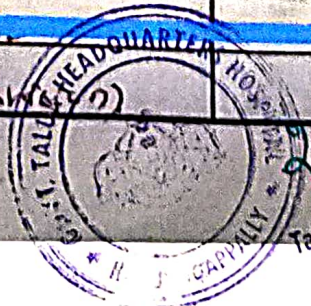

Superintendent
Taluk Head Quarters Hospital
Karunagappally, Kollam

PSO →

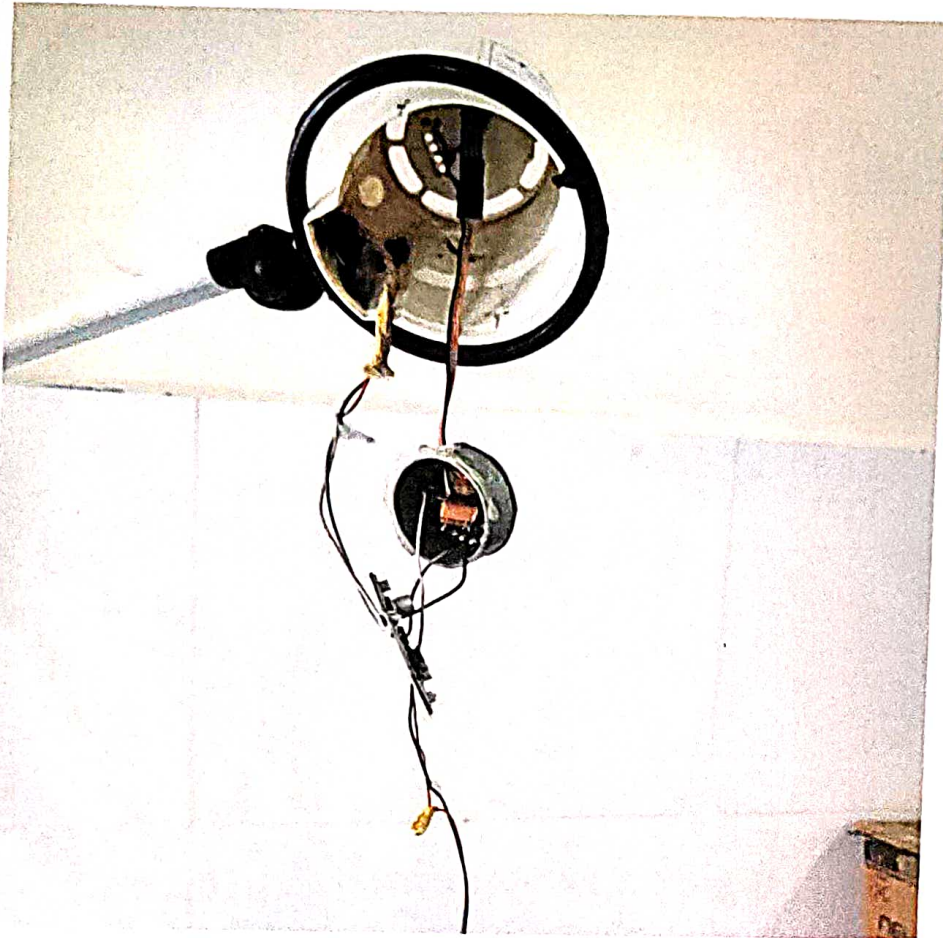

VRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)
KARUNAGAPALLY

TOLL FREE NO:1800 - 425-7669

BAR CODE - (8004-890615225)
0220458



MANUFACTURED BY

Hardik Medi Tec

E-mail : anand_medical@yahoo.com

Model No. : SPARX LED F004

Serial No. : SL/18-19/025

Item Name : MOBILE SPOT LIGHT



Superintendent
Taluk Head Quarters Hospital
Karunagappally, Kollam