



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. :

223712

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility ... <u>F.H.C. Kottukal</u></p> <p>Address ... <u>Kottukal</u></p> <p><u>Thiruvananthapuram, Kerala</u></p> <p>Ph : ... <u>9400097166</u></p>	<p>Call Registration Date : ... <u>05/06/24</u></p> <p>Caller ID : ... <u>U5261</u></p> <p>Date of Visit : ... <u>06/06/24</u></p> <p>Asset No. : ... <u>0151165</u></p> <p>EQPT Name : ... <u>BP Apparatus Digital</u></p> <p>Manufacture ... <u>Inf</u> ... Model : ... <u>NR</u></p> <p>S. No. ... <u>NR</u> ... Dept. ... <u>OP</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : checked the machine and found control board and pump damaged

Action Taken : Need to replace control board and pump to check the further working condition of the machine

Completed Date : 06/06/24 Time : 12:00 p.m. Spare Required


Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Mohammed Syadh M</u>	<u>06/06/24</u>	<u>11:00 AM</u>	<u>12:00 PM</u>

Customer Remark Completed Pending

Service Engineer Name : Mohammed Syadh M Customer Name : Mini Rs
 Signature : [Signature] Signature : [Signature]
 Date : 06/06/24 Date : 6/6/2024
 Contact Number : 7293499127 Contact Number : 9400097166
 Designation : Nursing officer JIC
 Hospital Seal : [Seal]




MEDICAL OFFICER IN CHARGE
FAMILY HEALTH CENTRE, KOTTUKAL
KOTTUKAL P.O., THIRUVANANTHAPURAM 695

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	PHC KOTTUKAL
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : BP Apparatus Make : INFI Model : BSX515 Serial No : 20200403148
4	Equipment ID/ Barcode	115261/0151165
5	Date of purchase/ Year of manufacture/Installation Date	27/03/2020
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	05/06/2024 (Toll free)
9	Action taken	Checked and found control board and pump defective. Need to replace these spares for further checking and working condition of the equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	NOT AVAILABLE

13	Asset Value	1353/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	Not Available
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found control board and pump defective. The unit is installed on 27/03/2020 and covered upto 4+ years. Quotation not attached since the spares are not available in the market. So recommending the unit for condemnation
17	Name & Signature of CYRIX Authority	MOHAMMED SIYAD 


*Not mandatory #Based on the period of life and value as per the BER guidelines

* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Control board and pump defective. Since the required spares are not available, this can be considered as beyond repairable.

MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram



10.2.2024
Signature of JC BM (NHM)

Date: _____



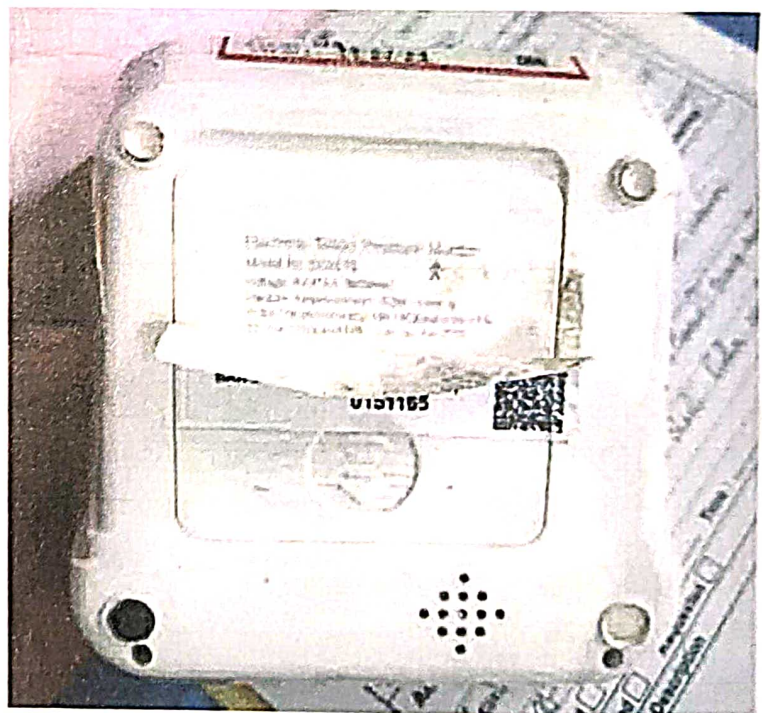

SUPERINTENDENT MEDICAL OFFICER IN CHARGE
FAMILY HEALTH CENTRE, KOTTUKKULAM
KOTTUKKULAM, PUNNAKKULAM
THIRUVANANTHAPURAM (74) - 695 501

20/8/19	12/15/19	from Kanna, ...	1		1	B
20/8/19	13/15/19	"	1		2	B
20/8/19	14/15/19	"	1		3	B
20/8/19	15/15/19	"	1		4	B
20/8/19	16/15/19	"	1		5	B
20/8/19	17/15/19	"	1		6	B
20/8/19	18/15/19	"	1		7	B
20/8/19	19/15/19	"	1		8	B
20/8/19	20/15/19	"	1		9	B
			1		10	B
(BNO. PW/DS/0818. Ps: 1119.19/1, Lifeline)						
5/5/19	21/15/19	from PHN		10	Nil	B
27/3/20	22/15/19	14/13 Tvm	2		2	B-TE50 N-1649
4/11/2020	23/15/19	FW stop Tvm	1		1	B
(Serial no: - CE0044, Mordiff)						
27/3/20		To OP		1	2	around Buna
20/4/22		To JHI (FNC admission)		1	1	B
18/11/22		To OP.		1	Nil	Shri. ... SR (F)
20.3.23		Physically found	2		2 also	
27.7.21		Issued a op Staff note Sub Stock page in (4)		2	Nil	B



MEDICAL OFFICER IN CHARGE
 FAMILY HEALTH CENTRE, KOTTUKAL
 KOTTUKAL P.O. PINNARAKKULAM
 THIRUVANANTHAPURAM - 695501
 THIRU

[Handwritten signature]
 DR. ...
 for MO etc.



Dr. K. Raji
for M.O. H.C.

MEDICAL OFFICER IN CHARGE
FAMILY HEALTH CENTRE, KOTTUKAL
KOTTUKAL P.O., PUNNAKKULAM
THIRUVANANTHAPURAM - 695 50