



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 223813

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

Health Facility : <u>CHC</u>	Call Registration Date : <u>25/05/24</u>
Address : <u>Anchuthengu</u>	Caller ID : <u>113214</u>
<u>Thiruvananthapuram</u>	Date of Visit : <u>26/05/24</u>
Ph : <u>7902375700</u>	Asset No. : <u>0130192</u>
	EQPT Name : <u>UPS</u>
	Manufacture : <u>Hykon</u> Model : <u>na</u>
	S. No. <u>200701287</u> Dept. <u>Laboratory</u>

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not working

Action Taken : checked and found that the inverter PCB, control PCB and 12V 7Ah battery defective. Need to replace these spares for further checking and working condition of the equipment spare Enquired with Vendor

Completed Date : 26/05/24 Time : 11:15 am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
<u>Vishnu. k</u>	<u>26/05/24</u>	<u>9.45 am</u>	<u>11.15 am</u>

Customer Remark : ബാറ്ററിയുടെ ആഫീസർ ഇൻചാർജ് സാമൂഹികാരോഗ്യകേന്ദ്രം അഞ്ചുതെങ്ങ് പി.ഒ. തിരുവനന്തപുരം - 695309

Completed Pending

Service Engineer Name : Vishnu.k
 Signature : [Signature]
 Date : 26/05/24
 Contact Number : 9605884413


Customer Name : [Signature]
 Signature : [Signature]
 Date : 26/5/24
 Contact Number : 7902375700
 Designation : Lab Tech Gr II
 Hospital Seal : [Seal]

**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	THIRUVANANTHAPURAM
2	Name of Hospital	CHC ANCHUTHENGU
3	Name of Equipment with Make, Model and Serial Number	Equipment Name : UPS 1KV. Make : HYKON Model : Green Bio 900 Serial No : 200701287
4	Equipment ID/ Barcode	113214/0130192
5	Date of purchase/ Year of manufacture/Installation Date	02/07/2020
6	Warranty details (Yes/No)	No Warranty
7	*AMC/ CAMC Period agreed at the time of purchase	No CAMC/AMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	25/05/2024
9	Action taken	Checked and found that the inverter PCB,Control PCB and 12v 7Ah battery defective.Need to replace these spares for further checking and working condition of the equipment.Enquired spare with vendor.
10	Present status of the equipment (Fully damaged / partially damaged)	FULLY DAMAGED
11	Recommendations for repair (required service details)	NOT RECOMMENDING FOR REPAIR
12	Cost of spares (specify parts and cost)	1KVA 24V Inverter PCB - 4130/- 1KVA Control PCB - 2950/- 12v 7 Ah Battery (2Nos) - 2176/- Total=9256/-

13	Asset Value	4500/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	205%
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	CYRIX SERVICE REPORT AND VENDOR QUOTATION ATTACHED
16	Reasons for recommending the equipment as BER	Checked and found that the inverter PCB, Control PCB and 12v 7Ah battery defective. The unit was installed on 02/07/2020 and covered upto 4+ years. The repairing cost is 205%. As per the tender clause 5.3.14.1 Both criteria met. So recommending the unit for condemnation.
17	Name & Signature of CYRIX Authority	DEEPAK EM 

*Not mandatory


#Based on the period of life and value as per the BER guidelines

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Inverter PCB, Control PCB damaged. Repair cost is high. So as per tender conditions it can be BER.


MANEESHA MOHAN M.R.
Junior Consultant (Biomedical)
National Health Mission
Thiruvananthapuram


18-07-2024
Signature of JC BM (NHM)




Date:

മെഡിക്കൽ ഓഫീസർ ഇൻചാർജ്
സാമൂഹികാരോഗ്യകേന്ദ്രം
അഞ്ചുതെങ്ങ് പി.ഒ.
തിരുവനന്തപുരം-695309


Signature of
Superintendent/Medical Officer (i/c)

HAE MATOLOGY ANALYSER

	Receipt	Issue	Balance
2/07/2020	Received from Labx opps SFS Trade Apartments, Kumardapuram, medical college, Tvm, Invoice No: EB/1254.		
	Medonic M Series M 32B, Bt: 113607. Rate: 1,44,000.00/-	1 nos.	1 nos
	② Medonic M Series Lyse, Quent: RFI0 20 Ltrs (1504460) Bt: 2003-311 Exp: 13/mar/2023.	2 nos.	2 nos
	③ Medonic M Series Lyse, RFI0 5 Ltrs (1504461) Bt: 1910-231 Exp: 23/oct/2022	2 nos.	2 nos
	④ Green Bto 900/12V with 2 nos 7 AH Battery, Bt: 200413376	1 nos.	1 nos
	⑤ Printer Epson Lx310 Dotmatrix Bt: Q7D 408638	1 nos.	1 nos
5/7/2020	All items are issued to Lab Technicians.	nil.	nil.

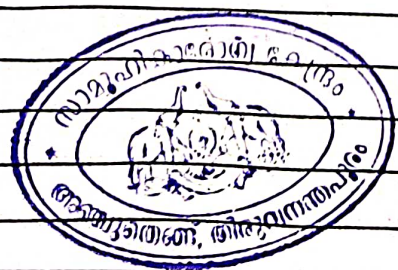

മെഡിക്കൽ ആഫീസർ ഇൻചാർജ്
സാമൂഹികാരോഗ്യകേന്ദ്രം
അഞ്ചുതെങ്ങ് പി.ഒ.
തമിഴുവനന്തപുരം-695309

[Handwritten signatures and initials in green ink]

AION BACKUPS

YP/VIII/320 AYLARA, KERALA KOLLAM

Date: 13/07/2024

Contact: 8921950217

Email: aionbackups12@gmail.com

GSTIN : 32CGUPM9450L1ZN


1KVA ONLINE UPS SERVICE PROPOSAL

TO,
CYRIX HEALTHCARE PVT. LTD
Barcode: 0130192
Ticket ID: 113214


Dear Sir/Madam,

We are pleased to submit here with our quote for the same as per below.

SL	DESCRIPTION	QTY	UNIT RATE IN INR	TOTAL	GST	TOTAL PRICE IN INR
1	1KVA 24V INVERTER PCB	1	3500.00	3500.00	18	4130.00
2	1KVA CONTROL PCB	1	2500.00	2500.00	18	2950.00
3	12v 7Ah Battery	2	850.00	1700.00	28	2176.00
PAYABLE AMOUNT						9256.00
Commercial terms and conditions 1. Payment 80% advance along with PO balance before dispatch, 20%After installation. 2. Delivery period; 2weeks. 3. Tax :GST@18% for spares, 28%@Battery 4. Installation; Our scope.						
Please arrange to release the PO at our above address						
Bank name :HDFC		Account no:50200082743176			IFSC Code:HDFC0004083	
We hope you will find the above offer in line with our discussions and await your valuable order please free to call or mail us on above given number if any query. Thank you, Sincerely, BHAGATH MOHAN						

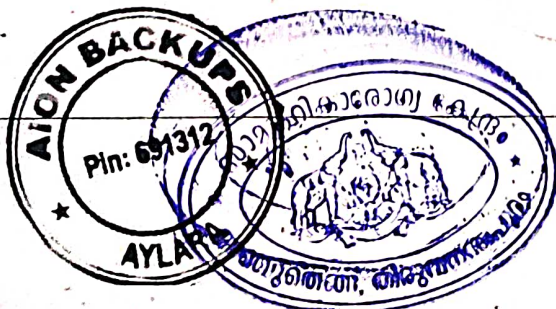

മെഡിക്കൽ ആഫീസർ ഇൻചാർജ്ജ്
സാമൂഹികാരോഗ്യകേന്ദ്രം
അഞ്ചുതെങ്ങ് പി.ഒ.
കുവന്തപുരം - 695309

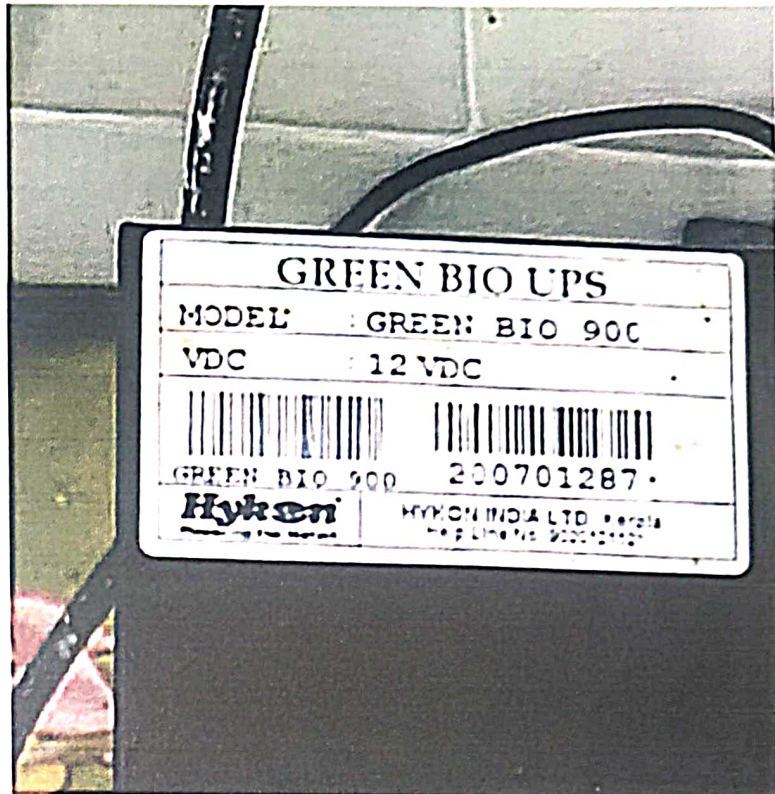

മെഡിക്കൽ ആഫീസർ ഇൻചാർജ്
 സാമൂഹികാരോഗ്യകേന്ദ്രം
 അടുത്തുതെങ്ങൽ പി.ഒ.
 തിരുവനന്തപുരം-695309



REGARDING QUOTATION FOR UPS-CHC ANCHUTENGU (0130192 0130178)

2 messages

Kasyep P V <kasyepcyrix@gmail.com>

Thu, 18 Jul 2024 at 10:02 pm

To: aionbackups12@gmail.com <aionbackups12@gmail.com>

Dear sir,

Kindly provide the service quotation for the 1 KV UPS at CHC Anchuthengu, Trivandrum

--

Thanks & Regards,

KASYEP PV

District Incharge , Trivandrum

CYRIX HEALTHCARE Pvt.Ltd

KLBEMP

Ph : +91 7593847134

kasyepcyrix@gmail.com

Bhagath Mohan <aionbackups12@gmail.com>

Thu, 18 Jul 2024 at 11:19 pm

To: Kasyep P V <kasyepcyrix@gmail.com>

Received your mail.

Thanks & Regards

Bhagath Mohan

PH:-8921950217

[Quoted text hidden]