


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KANNUR
2	Name of Hospital	PHC PATTIAM
3	Name of Equipment with Make, Model and Serial Number	BP APPARATUS Make: OMRON Model: HBP 1300 SN: NA
4	Equipment ID/ Barcode	1341133 #127153
5	Date of purchase/ Year of manufacture/Installation Date	10-03-2018 (Actual Installation date is 03.10.2018 Stock book copy attached for reference)
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free 03-08-2024
9	Action taken	Checked the Equipment found Equipment is not switching ON, found that Main Board, Pressure sensor and pump Defective. Need to replace these spare for further checking.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	2200/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report attached
16	Reasons for recommending the equipment as BER	Checked the Equipment found Equipment is not switching ON, found that Main Board, Pressure sensor and pump Defective. Need to replace these spare for further checking. In Ticket master Equipment installed on 10.03.2018. As per the stock book installation date is 03.10.2018 aged up to 05 years 10 months. Quotation not submitted since spares are not available in the market. So we recommending for condemnation.
17	Name & Signature of CYRIX Authority	AVINASH T 


*Not mandatory **#Based on the period of life and value as per the BER guidelines**

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:


Checked & identified that the machine not switching ON due to Main board, Pressure sensor and pump defective. Aged up to 5 years & above. Its service cost economically not feasible. So recommended for BER as per BER protocol.

Signature of JC BM (NHM)


 CONSULTANT BIOMEDICAL
 NATIONAL HEALTH MISSION
 KANNUR - 870002



Date: 23-8-24


 for Signature of
 Superintendent/Medical Officer (i/c)

COMMUNITY HEALTH CENTRE
 PATTIAM, CHERUVANCHERY



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 234841

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health FacilityPHC PATTIAM.....</p> <p>AddressPATTIAM.....</p> <p>.....KANNUR.....</p> <p>Ph :09203923523.....</p>	<p>Call Registration Date :03/8/2024.....</p> <p>Caller ID :127153.....</p> <p>Date of Visit :05/08/2024.....</p> <p>Asset No. :134.1133.....</p> <p>EQPT Name :B.P. Apparatus.....</p> <p>ManufactureOMRON..... Model :HBP1300.....</p> <p>S. No.NA..... Dept.OP.....</p>
---	--

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified :Equipment is not switching ON.....

Action Taken :Checked the equipment found equipment is not switching ON. Found that Main Barrel, Pressure sensor and pump Defective. Need to replace these spare for further checking.....

Completed Date : 05/08/2024 Time : 12:00pm Spare Required


Spare Replaced Requested



Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Prathyush T. Bragkari	05/08/2024	11:30am	12:00pm

Customer Remark Completed Pending

<p>Service Engineer Name : Prathyush T. Bragkari</p> <p>Signature : </p> <p>Date : 05/08/2024</p> <p>Contact Number : 9947025643</p>	<p>Customer Name : SISIRASIA</p> <p>Signature : </p> <p>Date : 5/08/2024</p> <p>Contact Number : 828127576</p> <p>Designation : N/O MEDICAL OFFICER</p> <p>Hospital Seal : COMMUNITY HEALTH CENTRE PATTIAM CHERUVANCHERY</p>
--	--

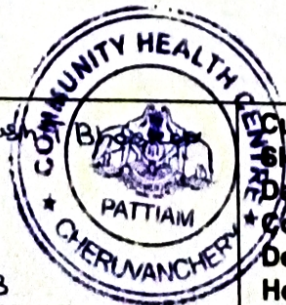

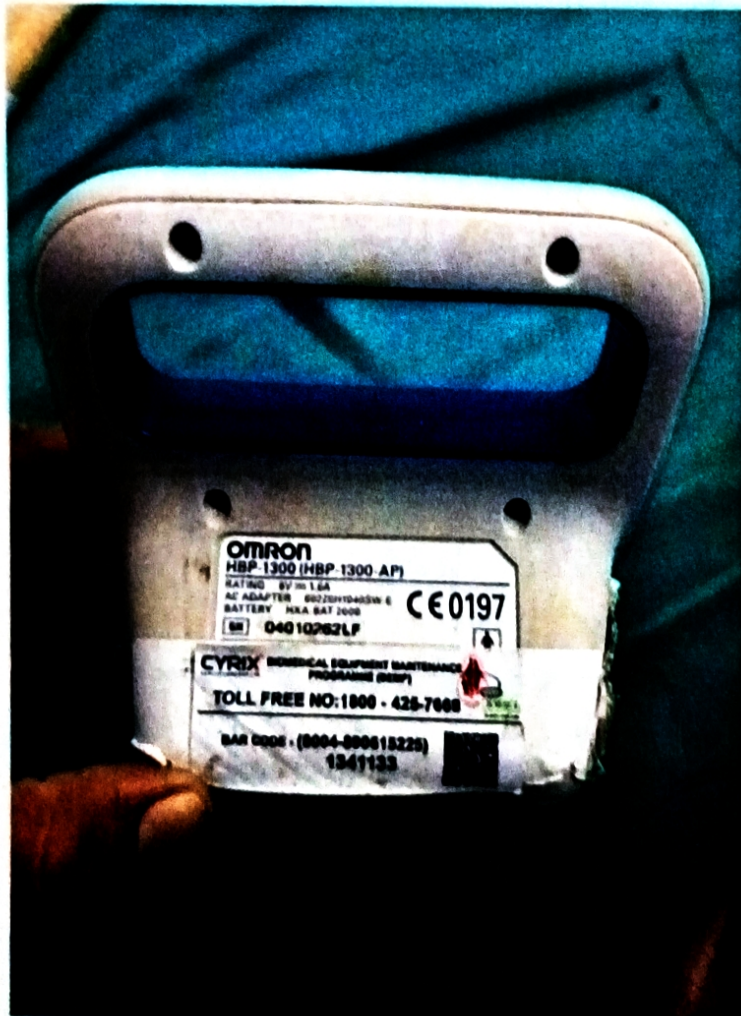

MEDICAL OFFICER
COMMUNITY HEALTH CENTRE
PATTIAM, CHERKUVANCHERY

22 BP APPARATUS

13/7/2009	Recd from store	2	2	
2/9/19	Transferred to amicable regt - Volume of P-3		2	recd
22.10.2006	Received from store (Local purchase)	1	1	
3/9/19	Transferred to amicable regt - Volume of P-3		1	recd
5/7/18	Recd from the store 70135219 (Barcode) (Kazunya) (Diamond)	2	2	Sub
5/7/18	Recd from pharmacy (Digital) 1350367 1350366	3	5	Sub
29/11/18	Recd from pharmacy (L.C.D Diamond)	2	7	Sub
3/10/18	Recd from pharmacy Com Reg # BP (Digital) (70133225 ³⁰⁰)	1	8	Sub
19/2/20	Transferred to Free Kottayam making (LCD Diamond)	2	2	6



23/9/24
 MEDICAL OFFICER
 COMMUNITY HEALTH CENTRE
 PATTIAM, CHERUVANCHERY