


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT  
MAINTENANCE PROGRAM (BEMP)**

**Recommendations for Beyond Economic Repair (BER)**

**PROFORMA**

<b>Sl. No</b>	<b>Particulars</b>	<b>Details</b>
1	Name of District	THRISSUR
2	Name of Hospital	PHC ANDATHODE
3	Name of Equipment with Make, Model and Serial Number	BP APPARATUS Make: ELKO Model: NIL SN: NIL
4	Equipment ID/ Barcode	0840653 #129545
5	Date of purchase/ Year of manufacture/Installation Date	Ticket master installation date-04-03-14 As per the stock book installation date is 15-04-2018
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free- 15-08-2024
9	Action taken	Checked the equipment and found board and display are defective. Need to replace these spares for further checking working condition of equipment.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA


13	Asset Value	1323 /-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Service report attached
16	Reasons for recommending the equipment as BER	Checked equipment found board and display are defective, In Ticket master installation date is 04-03-14. As per the stock book installation date is 15-04-2018 and covered up to 6 years and 4 months, Quotation not submitted since spares are not available in the market. So we recommending the equipment for condemnation.
17	Name & Signature of CYRIX Authority	BIJO T JOY 


\*Not mandatory **#Based on the period of life and value as per the BER guidelines**


\* Attach Photograph


Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

spares all not available.

  
Signature of JC BM (NHM)

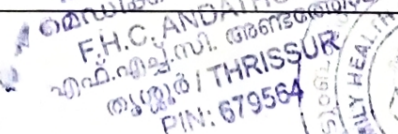

  
MEDICAL OFFICER  
F.H.C. ANDATHODU  
ANDATHODE - 679564  
PIN: 679564

  
Signature of Superintendent/Medical Officer (i/c)

Date: 27-08-24





# BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



**SERVICE PROVIDER**  
Tender No. WO-37/2021-2022/698

## CYRIX

HEALTHCARE PVT LTD

**No. :**  
224547

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

**Service Report** 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala  
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility ..... P.H.C.....</p> <p>Address ..... Andathacke..... Thoussar.....</p> <p>Ph : .....</p>	<p>Call Registration Date : ..... 15.08.2024.....</p> <p>Caller ID : ..... 129545.....</p> <p>Date of Visit : ..... 16.08.2024.....</p> <p>Asset No. : ..... 0840653.....</p> <p>EQPT Name : ..... Bp apparatus.....</p> <p>Manufacture ..... GLko ..... Model : ..... Nil.....</p> <p>S. No. ..... Nil..... Dept. ..... OP.....</p>
--	--

**Service Classification :** Breakdown Call  PMS  Calibration  Cust.Training

**Problem Identified :** ..... Not switching on.....

**Action Taken :** ..... checked the equipment and found board and display are defective. Need to repair these spares for further checking working condition of equipment.....

**Completed**  **Date :** 16.08.24 **Time :** 10:00am **Spare Required**

**Spare Replaced**  **Requested**

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrix Engineer	Date	Start Time	End Time
Byjo	16.08.24	9:00am	10:00am

**Customer Remark** **Completed**  **Pending**

<p><b>Service Engineer Name :</b> Byjo</p> <p><b>Signature :</b> </p> <p><b>Date :</b> 16.08.2024</p> <p><b>Contact Number :</b> 8981870060</p>	<p><b>Customer Name :</b> </p> <p><b>Signature :</b> </p> <p><b>Date :</b> 15/08/24</p> <p><b>Contact Number :</b> </p> <p><b>Designation :</b> Nirmalya of four</p> <p><b>Hospital Seal :</b> </p>
---	---



**CYRIX** BIOMEDICAL EQUIPMENT MAINTENANCE  
PROGRAMME (BEMP)



**TOLL FREE NO: 1800 - 425-7869**

BAR CODE - (8004-890615225)  
0840653



**ELKO**®

SYS.  
mmHg

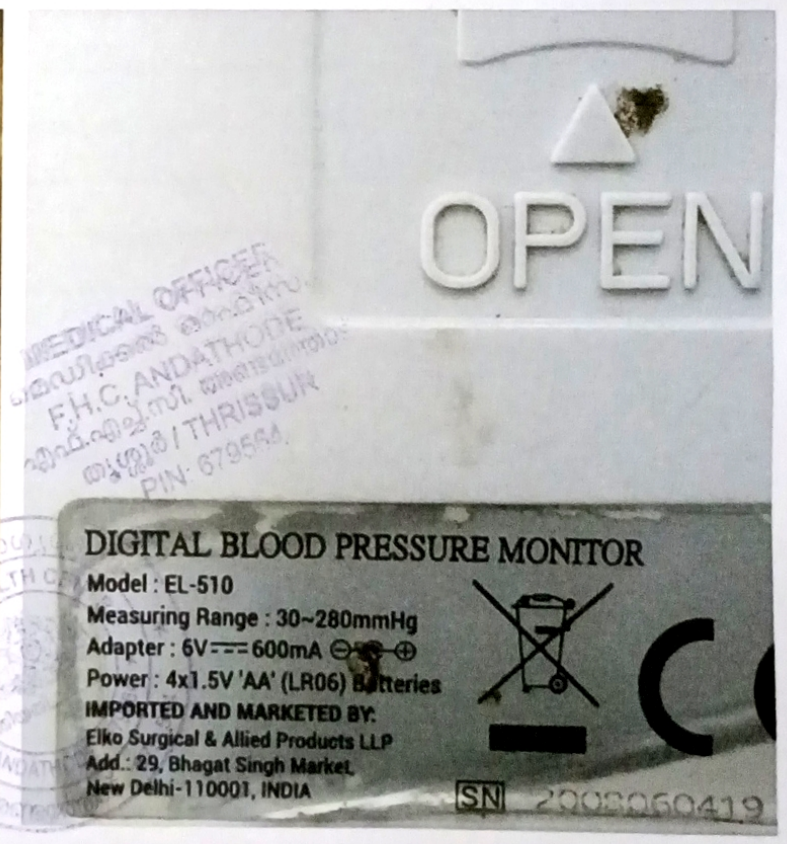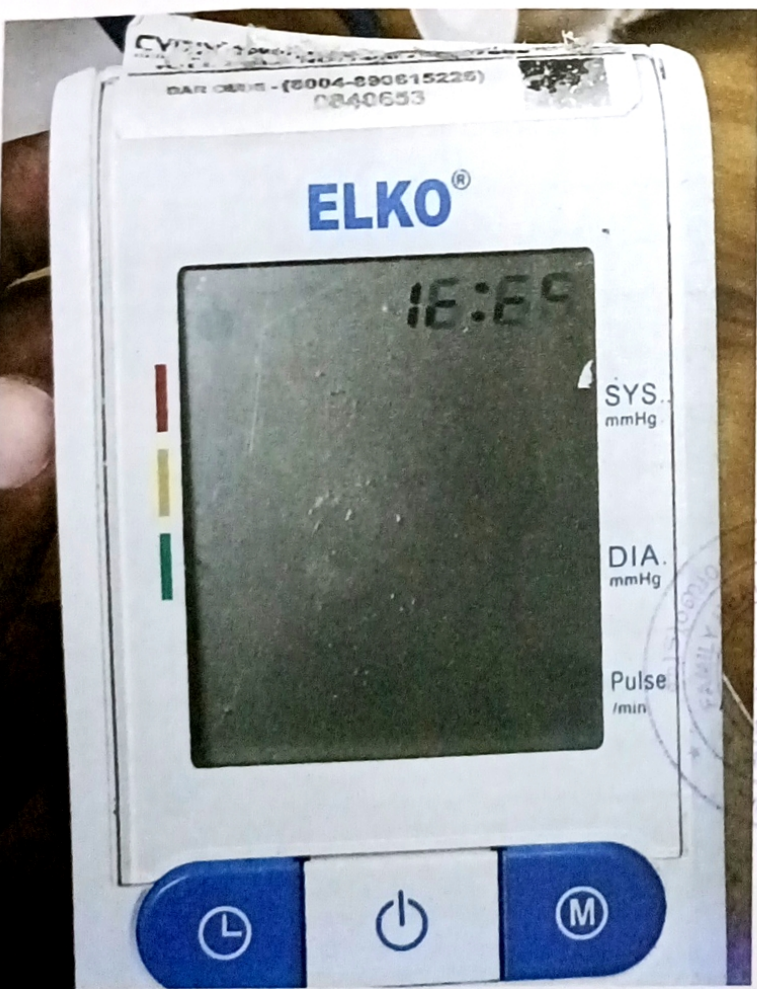



B.P Apparatus.

5/4/18. Ret ltrn Kauraya Community Phung

INNO: 594, dt: 12/1/18, P.No: 011, dt: 12/2005

mtg: UR, tab: 1875.00

24-5-18 Credit not no 43 dt 24.05.18 (Return back)

1 1 V  
NILU

