


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

| Sl. No | Particulars | Details |
|---------------|---|---|
| 1 | Name of District | KASARGOD |
| 2 | Name of Hospital | TH BEDADKA |
| 3 | Name of Equipment with Make, Model and Serial Number | LONG WAVE DIATHERMY MAKE: BIOTECH MODEL: STRIKER S/N: N/A |
| 4 | Equipment ID & Barcode | #118922, 1420333 |
| 5 | Date of purchase / Year of manufacture /Installation Date | 05-12-2018 |
| 6 | Warranty details (Yes/No) | NO WARRANTY |
| 7 | *AMC/ CAMC Period agreed at the time of purchase | NO AMC/CAMC |
| 8 | Date of breakdown(Date of registration of complaint through email/ Toll free) | 24-06-2024 (Toll free) |
| 9 | Action taken | Checked the machine, found problem with Applicator with lead for LWD, Disc for long wave, Power control PCB for LWD, Cabinet-LWD, Inactive electrode for LWD, Jelly for long wave, Main PCB for LWD. Enquired OEM for quotation. |
| 10 | Present status of the equipment (Fully damaged / partially damaged) | Not working, fully damaged. |
| 11 | Recommendations for repair (required service details) | Not recommending for repair |
| 12 | Cost of spares (specify parts and cost) | APPLICATOR WITH LEAD FOR LWD- 2800/- DISC FOR LONG WAVE- 6496/- POWER CONTROL PCB FOR LWD- 8850/- CABINET LWD- 4130/- INACTIVE ELECTRODE FOR LWD- 1848/- JELLY FOR LONG WAVE- 649/- MAIN PCB FOR LWD- 8555/- Total: 33328/- |

| | | |
|----|--|---|
| 13 | Asset Value | Ticket master asset value ₹67815 (As per the invoice asset value is 47978/- Invoice, Stock book attached for reference) |
| 14 | # Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value | 69.46% (with respect to cost of purchase-purchase bill & stock, detail attached for reference) |
| 15 | Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) | Cyrix service report and OEM quotation attached |
| 16 | Reasons for recommending the equipment as BER | After inspecting the machine, the following components were found defective: Applicator with lead for LWD, Disc for long wave, Power control PCB for LWD, Cabinet for LWD, Inactive electrode for LWD, Jelly for long wave, and Main PCB for LWD. The machine was installed on 05-12-2018 and is 5 years and 6 months old. The ticket master lists the asset value as 67,815/-, but the actual book value is 47,978/- (bills and stock details attached). The repair cost, based on the actual book value, is 69.46%, meeting both RBER criteria. As per tender clause 5.3.14.1, we recommend condemning the equipment. |
| 17 | Name & Signature of CYRIX Authority | ABHINAV O  |

*Not mandatory **#Based on the period of life and value as per the BER guidelines**

* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

Checked the machine and found problem with applicator with lead for LWD, Disc for long wave, power control PCB, for LWD, cabinet LWD, Inactive electrode for LWD, Jelly for longwave, & main PCB for LWD. Equipment installed on 05/12/2018. Repairing cost is above 69% of invoice asset value. Bill & stock details attached. Attached cyrix service report & quotation. So recommending the equipment for BER.

Jr. CONSULTANT
Biomedical Engineering
Arogyakeralam (NHM)
Kasaragod at Karhannad



Date

Seal

Signature of Superintendent / Medical Officer


ബോധധൂക്ക ഓഫീസർ
താലൂക്ക് ആശുപത്രി ബോധധൂക്ക
പി.ഒ. - 671541



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 209266

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | E-mail : bemp.kl@cyrix.in

| | |
|---|--|
| <p>Health Facility <u>Taluk Hospital</u></p> <p>Address <u>Bedadka</u> <u>Kasaragod</u></p> <p>Ph : <u>9747421257</u></p> | <p>Call Registration Date : <u>24.06.2024</u></p> <p>Caller ID : <u>118922</u></p> <p>Date of Visit : <u>25.06.2024</u></p> <p>Asset No. : <u>1420333</u></p> <p>EQPT Name : <u>Long Wave Diathermy</u></p> <p>Manufacture <u>Biotech</u> Model : <u>Staker</u></p> <p>S. No. <u>NA</u> Dept. <u>Physiotherapy</u></p> |
|---|--|

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Output not getting.

Action Taken : Checked the machine and found problem with machine mainboard, Power control PCB, Applicator, Disc and electrode. Need to replace these spares for further servicing of the equipment.


Completed Date : 25.06.24 Time : 2:30pm Spare Required

Spare Replaced Requested

| Description | Qty. | Part Number | PR Number |
|-------------|------|-------------|-----------|
| 1. | | | |
| 2. | | | |
| 3. | | | |


| Cyrix Engineer | Date | Start Time | End Time |
|------------------|-----------------|---------------|---------------|
| <u>Abhinav.D</u> | <u>25.06.24</u> | <u>1.30pm</u> | <u>2.30pm</u> |

Customer Remark Pending


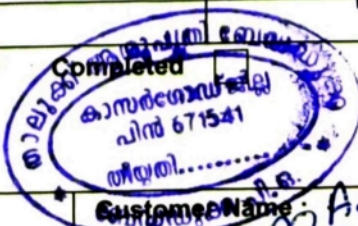


| | |
|---|---|
| <p>Service Engineer Name : <u>Abhinav.D</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>25.06.2024</u></p> <p>Contact Number : <u>8943392989</u></p> | <p>Customer Name : <u>Amalajyoti</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>25/6/24</u></p> <p>Contact Number : <u>9747421257</u></p> <p>Designation : <u>Physio</u></p> <p>Hospital Seal :</p> |
|---|---|

ഹെൽത്ത് കൗൺസിലർ ഓഫീസ്
 കൗൺസിലർ ഓഫീസ്
 ഫോൺ 671541

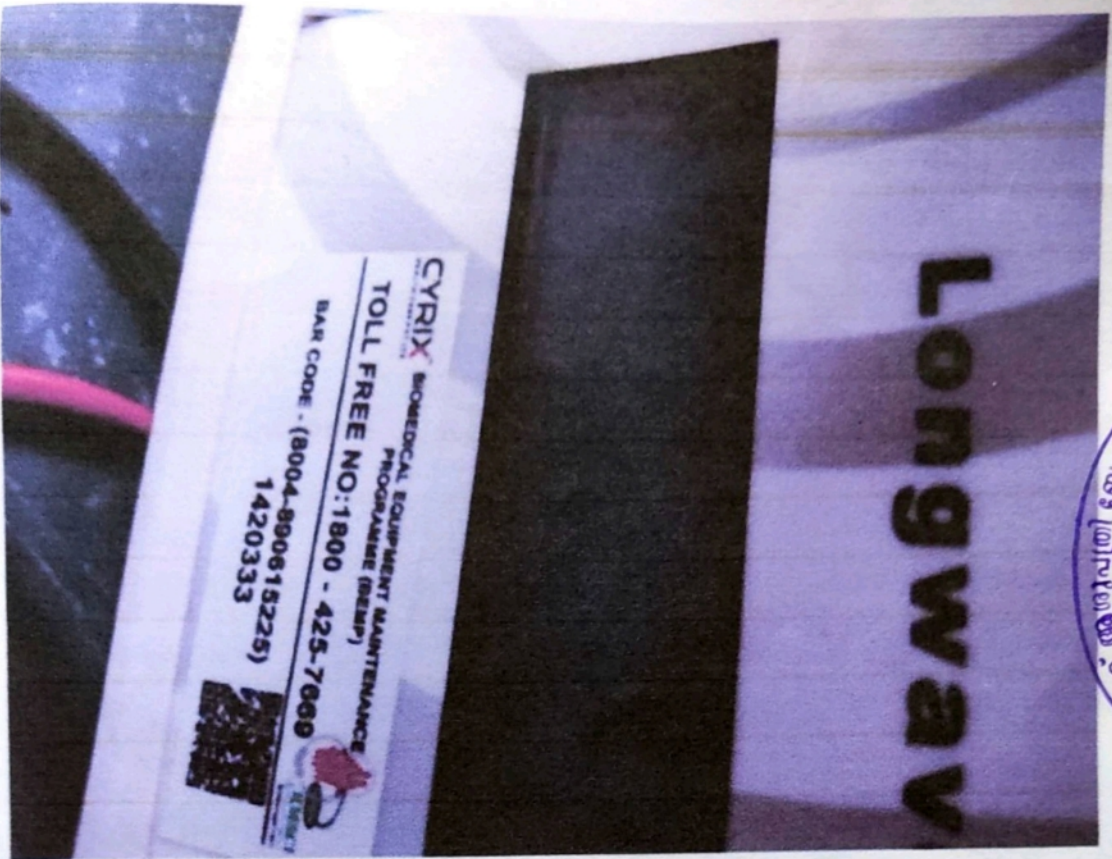

കേരള ശ്വേതം
 141519-ക-പി
 കോടംശ്വേതം
 കോടംശ്വേതം

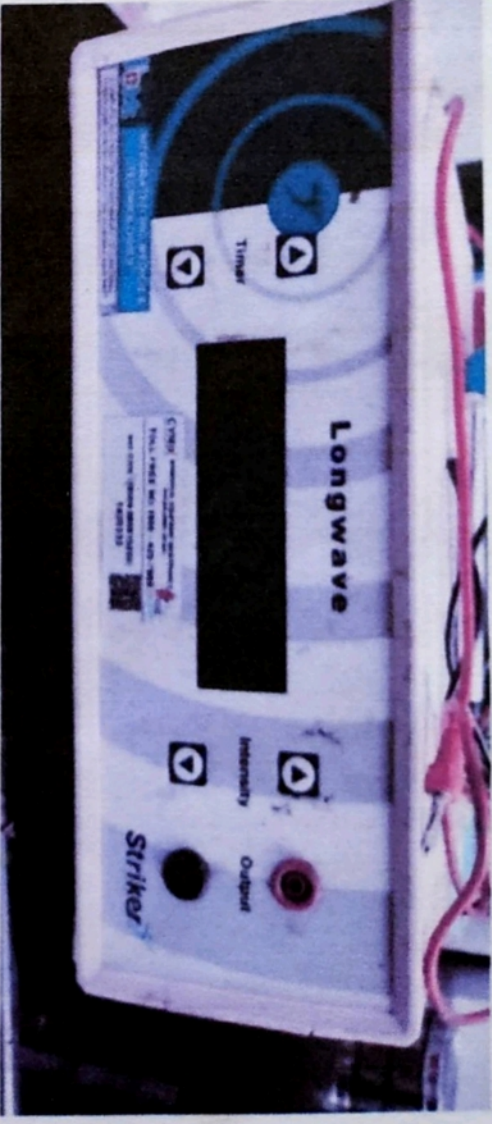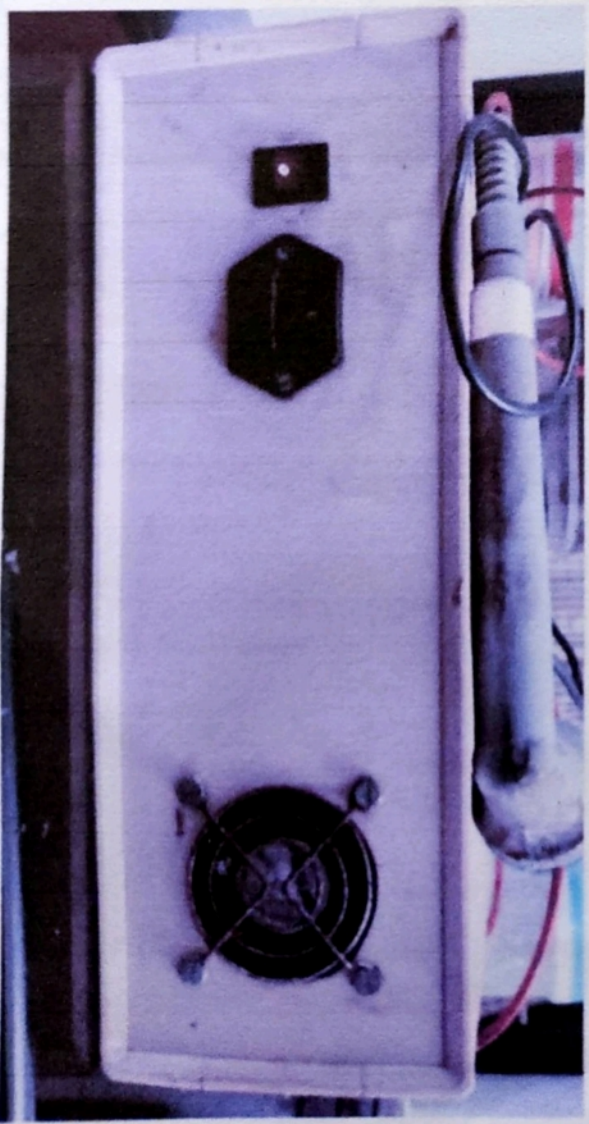

കേരള ശ്വേതം
 141519-ക-പി
 കോടംശ്വേതം
 കോടംശ്വേതം

Estimate

Estimate For

Cyrix Healthcare Pvt Ltd

FIRST FLOOR, 30/641B
PETTA JUNCTION,
POONITHURA, ERNAKULAM-682038,
KERALA INDIA

GSTIN : 32AAFCC2499H2ZM

State: 32-Kerala

Estimate Details

Estimate No. : MT/QT/24-25/106

Date : 10-07-2024

Place of supply: 32-Kerala

| # | Item name | Item Code | HSN/ SAC | Quantity | Unit | Price/ Unit | GST | Amount |
|---|---|-------------|-------------|----------|------|----------------|---------------------|--------------------|
| 1 | Applicator withlead for LWD | 09114 | 90189099 | 1 | Pcs | ₹ 2,500.00 | ₹ 300.00 (12%) | ₹ 2,800.00 |
| 2 | Disc for Longwave (45mm) | 09138 | 90189099 | 1 | Pcs | ₹ 5,800.00 | ₹ 696.00 (12%) | ₹ 6,496.00 |
| 3 | Power control Pcb for LWD (Power control unit for LWD) | 38635308992 | 90189099 | 1 | - | ₹ 7,500.00 | ₹ 1,350.00 (18%) | ₹ 8,850.00 |
| 4 | Cabinet- LWD (Cabinet for LWD) | 3866338792 | 90189099 | 1 | - | ₹ 3,500.00 | ₹ 630.00 (18%) | ₹ 4,130.00 |
| 5 | Inactive Electrode for LWD (Inactive Electrode with lead for LWD) | 09113 | 90189099 | 1 | - | ₹ 1,650.00 | ₹ 198.00 (12%) | ₹ 1,848.00 |
| 6 | Jelly For Longwave ((250 ml)) | 09105 | 90181290 | 1 | Nos | ₹ 550.00 | ₹ 99.00 (18%) | ₹ 649.00 |
| 7 | Main Pcb for LWD (Modified Pcb for LWD) | 38661902279 | 90189099 | 1 | - | ₹ 7,250.00 | ₹ 1,305.00 (18%) | ₹ 8,555.00 |
| 8 | Freight Charges | FREIGHT | 48195010 | 1 | - | ₹ 900.00 | ₹ 162.00 (18%) | ₹ 1,062.00 |
| | Total | | | 7 | | | ₹ 4,740.00 | ₹ 34,390.00 |



Jayesh Krishnan <jayeshcyrix@gmail.com>

MACHINE SENT FOR SERVICE - LONGWAVE DIATHERMY - BARCODE 1420333

12 messages

Abhinav O <abhinavcyrix@gmail.com>

Thu, Jun 27, 2024 at 9:00 AM

To: MURALIKRISHNA S <muralikrishnaalpy@gmail.com>

Cc: Jayesh Krishnan <jayeshcyrix@gmail.com>, Sarang KM <sarangcyrix@gmail.com>

Dear sir,

This mail is to inform you that as per our telephonic conversation I had sent the Long Wave diathermy machine and probe to your address for service on 26/06/2024. Please find the courier details attached below and do the needful at the earliest.

Thanks & Regards

Abhinav O

Cyrix Healthcare Pvt. Ltd

Kasaragod | Kerala

Mob:8943392989

**IMG_20240626_104839.jpg**
3945K**Jayesh Krishnan** <jayeshcyrix@gmail.com>

Mon, Jul 1, 2024 at 10:26 AM

To: MURALIKRISHNA S <muralikrishnaalpy@gmail.com>

Cc: Sarang KM <sarangcyrix@gmail.com>, Abhinav O <abhinavcyrix@gmail.com>, DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <zm2.klbemp@cyrix.in>

Dear sir,

Kindly update the status of service.

[Quoted text hidden]

--

Thanks & Regards

JAYESH KRISHNAN,

Sr. Biomedical Engineer,

District In-charge

Kasaragod.

PH:- 7593847156

jayeshcyrix@gmail.comwww.cyrixhealthcare.com**Cyrix Healthcare Pvt Ltd****| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India****KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH****Jayesh Krishnan** <jayeshcyrix@gmail.com>

Thu, Jul 4, 2024 at 10:15 AM

To: MURALIKRISHNA S <muralikrishnaalpy@gmail.com>

Cc: Sarang KM <sarangcyrix@gmail.com>, Abhinav O <abhinavcyrix@gmail.com>, DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <zm2.klbemp@cyrix.in>

Sir,
Kindly update urgently.
[Quoted text hidden]

MURALIKRISHNA S <muralikrishnaalpy@gmail.com> Wed, Jul 31, 2024 at 9:16 AM
To: Jayesh Krishnan <jayeshcyrix@gmail.com>
Cc: Sarang KM <sarangcyrix@gmail.com>, Abhinav O <abhinavcyrix@gmail.com>, DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <zm2.klbemp@cyrix.in>

Dear Sir/ Madam,

Kindly find the attached quotation.

--
Thanks and Regards


Muralikrishna Suresh
Sales & Service Manager

Whatspp: <https://wa.me/919074126766>

[Quoted text hidden]

--

[Quoted text hidden]

 **Estimate_MT QT 24-25 115_27_07_24.pdf**
108K