


**REPAIR OF BIOMEDICAL EQUIPMENTS UNDER BIOMEDICAL EQUIPMENT
MAINTENANCE PROGRAM (BEMP)**

Recommendations for Beyond Economic Repair (BER)

PROFORMA

Sl. No	Particulars	Details
1	Name of District	KANNUR
2	Name of Hospital	PHC EZHOME
3	Name of Equipment with Make, Model and Serial Number	BP APPARATUS Make: OMRON Model: HEM 7121 SN: 2017100132VGI
4	Equipment ID/ Barcode	1342576 #127227
5	Date of purchase/ Year of manufacture/Installation Date	20-06-2019 (Actual Installation date is 04.08.2021 Stock book copy attached for reference)
6	Warranty details (Yes/No)	No warranty
7	*AMC/ CAMC Period agreed at the time of Purchase	No AMC/CAMC
8	Date of breakdown (Date of registration of complaint through email/ Toll free)	Toll free 03-08-2024
9	Action taken	Checked the Equipment found Equipment is not switching ON, found that Main Board, Pressure sensor and pump Defective. Need to replace these spare for further checking.
10	Present status of the equipment (Fully damaged / partially damaged)	Fully damaged
11	Recommendations for repair (required service details)	No recommendations
12	Cost of spares (specify parts and cost)	NA

13	Asset Value	2200/-
14	# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value	NA
15	Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not)	Cyrix Service report attached
16	Reasons for recommending the equipment as BER	Checked the Equipment found Equipment is not switching ON, found that Main Board, Pressure sensor and pump Defective. Need to replace these spare for further checking. In software Equipment installed on 20.06.2019. As per the stock book installation date is 04.08.2021 aged up to 03 years. Quotation not submitted since spares are not available in the market. So we recommending for condemnation.
17	Name & Signature of CYRIX Authority	AVINASH T 


*Not mandatory

#Based on the period of life and value as per the BER guidelines


* Attach Photograph

Remarks and Recommendations of Junior Consultant (Biomedical) NHM:

checked & identified that machine not switching ON, due to main board, Pressure sensor, Pump are defective. The spare cost economically not feasible. Aged up to 3 years. Be recommended for BER as per BER protocol.

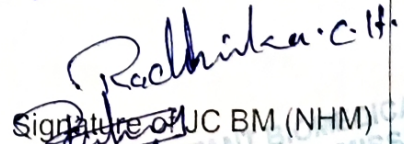

 Rachika C. K.
 Signature of Junior Consultant (Biomedical) NHM
 30/08/2024
 NATIONAL HEALTH MISSION
 KANNUR - 670002

Haashida. K


 Nursing Officer

Date: 31/8/24




 Superintendent/Medical Officer (i/e)
 0497 2815163



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 230468

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report 30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

<p>Health Facility <u>PHC EZHOME</u></p> <p>Address <u>EZHOME</u> <u>KANNUR</u></p> <p>Ph : <u>8589867067</u></p>	<p>Call Registration Date : <u>3/8/24</u></p> <p>Caller ID : <u>127227</u></p> <p>Date of Visit : <u>4/8/24</u></p> <p>Asset No. : <u>1342576</u></p> <p>EQPT Name : <u>BP Apparatus</u></p> <p>Manufacture <u>Omron</u> Model : <u>HEM7124</u></p> <p>S. No. <u>20171000132491</u> Dept. <u>OP</u></p>
---	---

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Not switching ON.

Action Taken : checked the equipment found equipment is not switching on. found that main board, pressure sensor and pump defective. Need to replace these spares for further checking.

Completed Date : 4/8/24 Time : 11:40am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			

Cyrlix Engineer	Date	Start Time	End Time
<u>Aswin</u>	<u>4/8/24</u>	<u>10:50am</u>	<u>11:40am</u>

Customer Remark Completed Pending

(Handwritten notes in Malayalam)

Service Engineer Name : Aswin

Signature : *(Signature)*

Date : 4/8/24

Contact Number : 8301012759

Customer Name : Harshida.K

Signature : *(Signature)*

Date : 4/8/24

Contact Number : 8914517173

Designation : Nursing Officer

Hospital Seal : *(Seal)*


Brought from stock register vol. I p. no 74.
192 Digital BP Apparatus.

Date		Receive NO	Issue NO	Balance
4/8/21	Received from the store. (From CLTC Ayurveda Pamyanam)	1		1
21/12/21	Received from the store. [Mercury free type (NCD Supply)]	2		3
C/O to stock register of equipments p. no 749.				

Flashida. K
~~hater~~

Nursing officer.



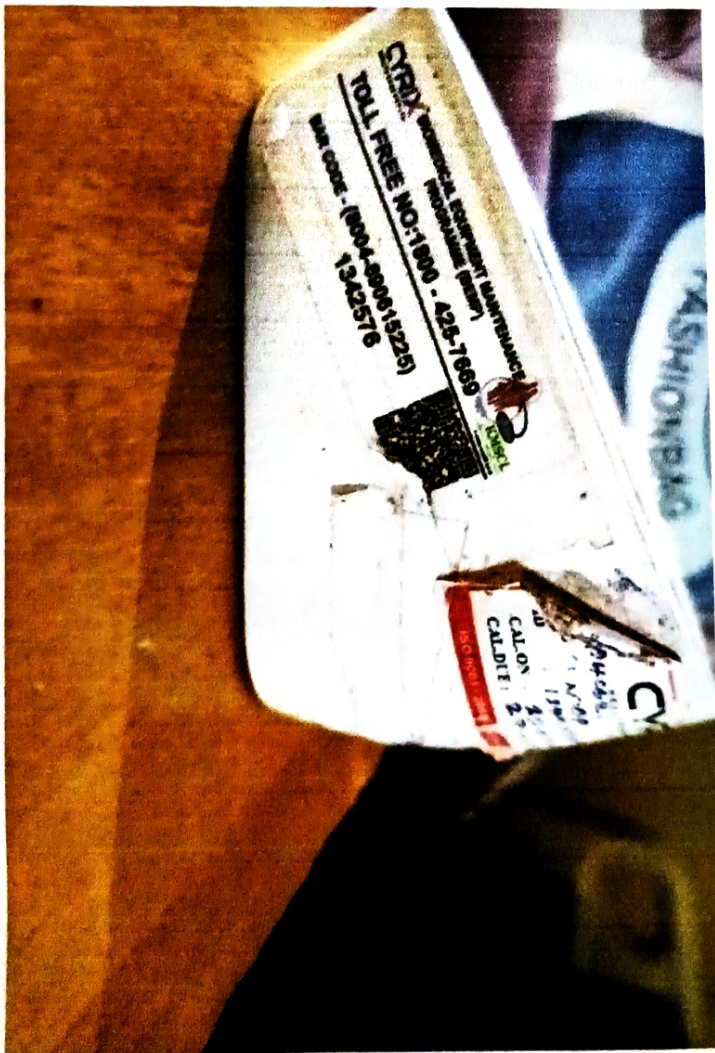

Harshida K
Woty

Nursing Officer

