

PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)

Name of Hospital: PHC VELUR	Name of District: Thrissur
Name of Equipment: Nebulizer	Equipment ID & Barcode: 130761 & 0840870
Make: Life Care	Model: CNB69022
Serial Number: LC22190401770	Warranty details: No Warranty
Date of purchase/Year of manufacture/ Installation Date: Ticket master installation date - 06-08-2018 As per the Stock book installation date - 06-08-2019	Present status of the equipment: Fully damaged
Date of breakdown: 22-08-2024 Date of registration of complaint through email/ toll free): Toll free	*AMC/ CAMC Period agreed at the time of purchase: No AMC/CAMC
Action taken: Machine checked and found motor and piston are defective. Need to replace these spares for working condition of equipment.	


Recommendations for repair (required service details) - Not recommending for repair

Cost of spares (specify parts and cost): N/A


# Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: N/A	Asset Value: 1353/-
---------------------------------------------------------------------------------------------	---------------------

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not) - Cyrix service report attached

Reasons for recommending the equipment as BER: checked the machine and found piston and motor are defective. In ticket master installation date is 06-08-2018, As per the stock book installation date is 06-08-2019 aged up to 5 years. Quotation not submitted since spares are not available from the market. So we recommending the equipment for condemnation.

BIJO T JOY 
 Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Nebuliser's piston and motor are complaint. Spare not available

Recommended for BER (Yes/ No): <i>yes</i>	 Signature of JC BM (NHM) <i>[Signature]</i> 21/8/24
Date: <i>2/9/24</i>	


 Signature of Superintendent / Medical Officer (i/c)

Date: _____

*Not mandatory # Based on the period of life and value as per the BER guidelines * Attach Photograph



ബിജിട് ജോയ്
 ജൂനിയർ കൺസൾട്ടന്റ് (ബയോമെഡിക്കൽ) NHM, തൃശ്ശൂർ



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

No : 1000294

CYRIX[®]

HEALTH CARE PVT LTD

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi- 682 038, Kerala
Ph : 98472 99500 Website : www.cyrix.com | Email : bemp.kl@cyrix.in

<p>Health Facility..... <u>PHC</u>.....</p> <p>Address..... <u>Velud</u>.....</p> <p style="padding-left: 40px;"><u>Thirissur</u></p> <p>Ph:..... <u>974625660</u>.....</p>	<p>Call Registration Date : <u>22-08-2024</u>.....</p> <p>Caller ID : <u>130761</u>.....</p> <p>Date of Visit : <u>23-08-2024</u>.....</p> <p>Asset No : <u>0840870</u>.....</p> <p>EQPT Name : <u>Nebulizer</u>.....</p> <p>Manufacture..... <u>Life Care</u>..... Model: <u>CN369022</u></p> <p>S. No. <u>Lc2219041770</u>..... Dept..... <u>OP</u></p>
-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Service Classification : Breakdown call PMS Calibration Cust. Training

Problem Identified : not working the motor

Action Taken : machine checked and found piston and motor are defective need to replace these spares for working condition of equipment

Completed Date : 23-08-2024 Time : 11:00am Spare Required

Spare Replaced Requested

Description	Qty.	Part Number	PR Number
1.			
2.			
3.			




Cyrix Engineer	Date	Start Time	End Time
<u>Biyo</u>	<u>23-8-24</u>	<u>10:00am</u>	<u>11:00am</u>

Customer Remark Completed Pending

Service Engineer Name : Biyo
Signature: [Signature]
Date: 23-08-2024
Contact Number: 8921970010



Customer Name : Salmath
Signature: [Signature]
Date: 23/8/2024
Contact Number:
Designation : [Signature]
Hospital Seal

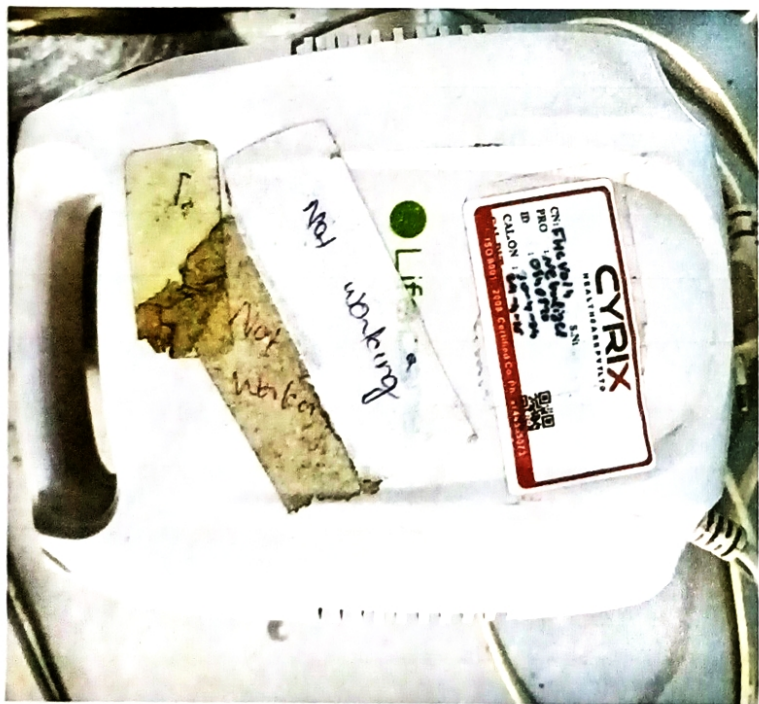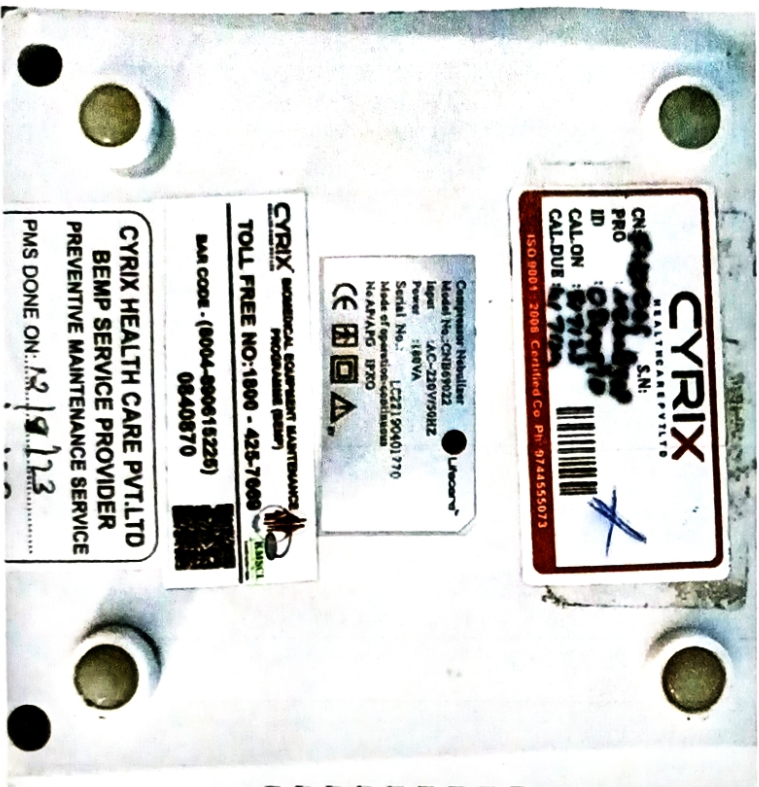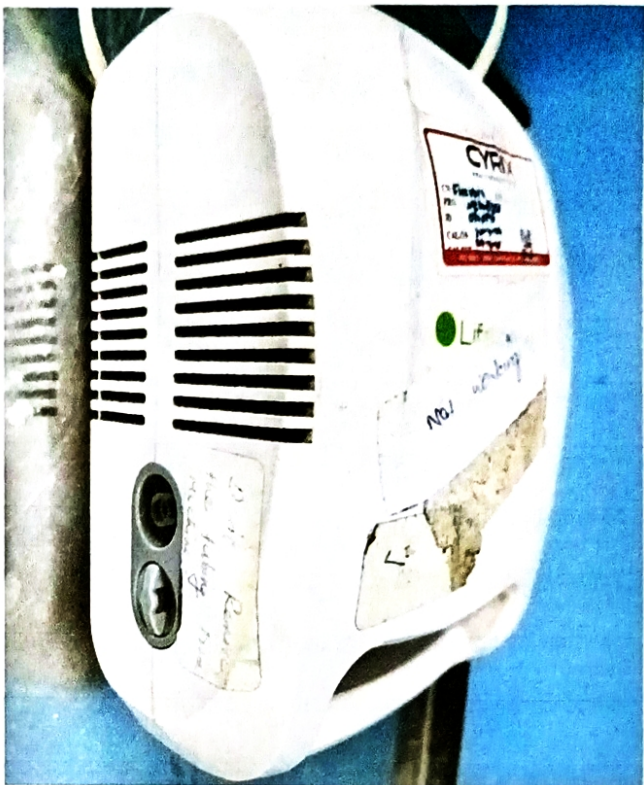

NEBULISER

Date	Item	Qty from store	issue	Balance	Signs
20/05/18	Nebuliser - adult and paediatric	1	OP	ND	d ₂
d	mask kit life line compress nebuliser		(damaged and moved to (unusable))		junk room
21/12/18	Nebuliser	1			
6/8/19	Nebuliser	1			
2/4/24	Nebuliser (OMRON) ne-C28		received from pharmacy store		
	OMRON health care 1		(3349.92)		

