

**PROFORMA
RECOMMENDATION FOR BEYOND ECONOMIC REPAIR (RBER)
BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAM (BEMP)**

| | |
|---|---|
| Name of Hospital: THQH KUTTIADI | Name of District: KOZHIKODE |
| Name of Equipment: CENTRIFUGE | Equipment ID & Barcode: 125383 & 1120685 |
| Make: KEMI | Model: C8C |
| Serial Number: 14017 | Warranty details: NO Warranty |
| Date of purchase/ Year of manufacture/ Installation Date: TICKET MASTER INSTALLATION DATE IS 03/07/2008, AS PER STOCK BOOK INSTALLATION DATE IS 21/06/2005 (STOCK BOOK ATTACHED FOR REFERENCE) | Present status of the equipment: Fully damaged |
| Date of breakdown: 25/07/2024 Date of registration of complaint through email/ Toll free): Toll free | *AMC/ CAMC Period agreed at the time of purchase: NO AMC/CAMC |
| Action taken: Checked and found equipment not switching on, found main board with display and motor defective. Enquired spares with oem | |

Recommendations for repair (required service details): Not recommending for repair

Cost of spares (specify parts and cost): 1) Sticker & Control board set for c8c centrifuge -1 nos = 3000/-
2) Motor for c8c centrifuge - 1 nos = 3200 /-
TOTAL = 6200 /-
GST = 1116/-
GRAND TOTAL = 7316 /-

| | |
|--|---------------------|
| # Percentage value of the cost of spares with respect to Cost of Purchase/ Asset Value: 75.80% | Asset Value: 9651/- |
|--|---------------------|

Abstract of Service Report provided by the OEM/ Authorized Service Provider/ CYRIX (Attached or Not): Cyrix service report attached and vendor quotation attached

Reasons for recommending the equipment as BER: Checked and found equipment not switching on, found main board with display and motor defective. In Ticket master installation date is 03/07/2008, As per stock book installation date is 21/06/2005 (stock book attached for reference). Equipment out lived 19 years 2 months. Spare cost of the equipment is 75.80% both criteria for RBER met, As per tender clause 5.3.14.1 we recommending the equipment for condemnation.


JINEESH PP
Name & Signature of CYRIX Authority with date

Remarks of Junior Consultant (Biomedical) NHM:
Checked and found that equipment is not switching on. Main board with display and motor damaged. Machine is installed on 3/7/2008. Spare cost is high. So recommended for condemnation.

| | |
|--|---|
| Recommended for BER (Yes/ No): Yes <input checked="" type="checkbox"/> | Consultant Bio Medical Engineer National Health Mission Kozhikode Signature of JC BM (NHM) |
| Date: 29/08/2024 | |

| | | |
|-------|------|---|
| Date: | Seal | Signature of Superintendent / Medical Officer (c) |
|-------|------|---|

*Not mandatory #Based on the period of life and value as per the BEMP guidelines. Attach Photograph

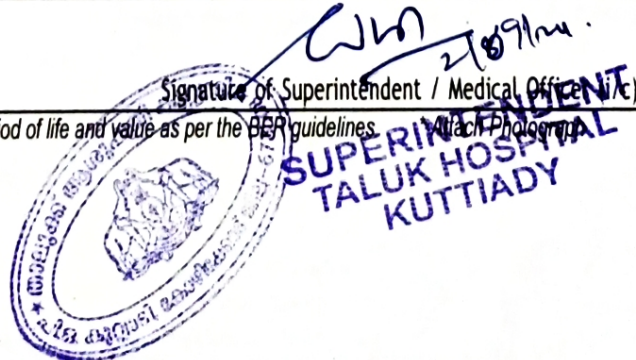



BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME UNDER NATIONAL HEALTH MISSION



SERVICE PROVIDER
Tender No. WO-37/2021-2022/698

CYRIX

HEALTHCARE PVT LTD

No. : 234981

ISO 13485 : 2012 & ISO 9001-2008 CERTIFIED COMPANY | AERB Approved Service Agency

Service Report

30/64 1 B, Petta Junction, Poonithura, Kochi - 682 038, Kerala
Ph : 98472 99500 Website : www.cyrrix.com | E-mail : bemp.kl@cyrix.in

| | |
|--|---|
| <p>Health Facility : <u>TH</u></p> <p>Address : <u>KUTTIADY</u> <u>KOZHIKODE</u></p> <p>Ph : <u>9349633603</u></p> | <p>Call Registration Date : <u>25/7/24</u></p> <p>Caller ID : <u>125383</u></p> <p>Date of Visit : <u>26/7/24</u></p> <p>Asset No. : <u>1120685</u></p> <p>EQPT Name : <u>Centrifuge</u></p> <p>Manufacture : <u>Kemi</u> Model : <u>C-8C</u></p> <p>S. No. <u>14017</u> Dept. <u>Lab</u></p> |
|--|---|

Service Classification : Breakdown Call PMS Calibration Cust.Training

Problem Identified : Machine not getting on.

Action Taken : Checked and Found the issue in main board, display, and motor is defective need to replace these spare for further checking and working condition of machine.

Completed Date : 26/7/24 Time : 8:50AM Spare Required


Spare Replaced Requested

| No. | Description | Qty. | Part Number | PR Number |
|-----|-------------|------|-------------|-----------|
| 1. | _____ | | | |
| 2. | _____ | | | |
| 3. | _____ | | | |

| Cyrrix Engineer | Date | Start Time | End Time |
|-----------------|----------------|---------------|---------------|
| <u>ARUNK K</u> | <u>26/7/24</u> | <u>8:00AM</u> | <u>8:50AM</u> |

Customer Remark _____ **Completed** **Pending**

| | |
|--|---|
| <p>Service Engineer Name : <u>ARUNK K</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>26/7/24</u></p> <p>Contact Number : <u>7593847164</u></p> | <p>Customer Name : <u>Alfath.k.h</u></p> <p>Signature : <u>[Signature]</u></p> <p>Date : <u>26/7/24</u></p> <p>Contact Number : <u>9349633603</u></p> <p>Designation : <u>Lab Technician</u></p> <p>Hospital Seal :</p> |
|--|---|

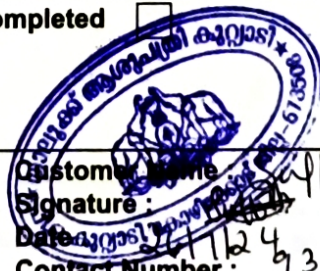


SUPERINTENDENT
TALUK HOSPITAL
KUTTIADY



FABI ASSOCIATES

FABI ASSOCIATES

GSTIN:32ACAPM3449H1ZV

| An associate concern of KEM! | | | | |
|--|--|---|------------------------------|---|
| PROFORMA INVOICE | | | | |
| Bill To, M/S.CYRIX HEALTHCARE PVT. LTD. FIRST FLOOR, PETTA JUNCTION 30/641B, POONITHURA, ERNAKULAM GSTIN/UIN: 32AAFCC2499H2ZM, State Name: Kerala, Code: 32, E-Mail: purchase.kl@cyrix.in | | NO | 270824 | |
| | | Date | 27 TH AUGUST 2024 | |
| | | Delivery | 3 Days, Against payment. | |
| | | Payment | Advance by Bank Transfer. | |
| Ref→ Your verbal order by phone call on 27-08-24. | | Our Bank & QR Code :- STATE BANK OF INDIA, VAZHAKULAM (MUDICKAL) BRANCH. ACCOUNT NO: 38381196927, IFS CODE:- SBIN 0070305 | |  |
| SI | Particulars | Qty | Value [Rs.] | Amount [Rs.] |
| 1. | SPARE-STICKER & CONTROL BOARD SET FOR C-8C-[CENTRIFUGE] | 1 | 3,000.00 | 3,000.00 |
| 2. | SPARE-MOTOR FOR C-8C-[CENTRIFUGE] | 1 | 3,200.00 | 3,200.00 |
| | | | TOTAL | 6,200.00 |
| | | | Add:GST@18% | 1,116.00 |
| | | | ROUND OFF | 0.00 |
| | | | Net Amount Payable | <u>7,316.00</u> |
| Amount (in words) : INR Seven Thousand Three Hundred & Sixteen Only /- | | | | |

NB: Kindly inform us through our E-Mail after transfer the payment.

For FABI ASSOCIATES

Authorized Signatory



EQUIRED SPARE QUOTATION -1120685 -125383 -CENTRIFUGE -THQH KUTTIADI ,KOZHIKODE, erala

messages

neesh P P <jineeshcyrix@gmail.com>
: moideenkemi@gmail.com
: DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <zm2.klbemp@cyrix.in>

Fri, 9 Aug, 2024 at 6:18 p

Dear Sir,

Please share price and spare availability of Main board with display and motor

Centrifuge
Make : KEMI (KADAVIL MECHANICAL INDUSTRIES)
Model: C8C
SN: 14017

Attached photos for your reference

Thanks & Regards,

Jineesh PP
District Incharge - Kozhikode
Mob-7593847163
jineeshcyrix@gmail.com
www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd

| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India

KERALA || KARNATAKA || TAMIL NADU || UTTAR PRADESH

neesh P P <jineeshcyrix@gmail.com>
: moideenkemi@gmail.com
: DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <zm2.klbemp@cyrix.in>

Mon, 12 Aug, 2024 at 8:36 a

Dear Sir,

Reminder
[Quoted text hidden]

neesh P P <jineeshcyrix@gmail.com>
: moideenkemi@gmail.com
: DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>, Blesson Jose <zm2.klbemp@cyrix.in>

Tue, 13 Aug, 2024 at 6:59 a


[Quoted text hidden]

OIDEEN KEMI <moideenkemi@gmail.com>
: Jineesh P P <jineeshcyrix@gmail.com>

Tue, 13 Aug, 2024 at 5:12 p

PLEASE CONTACT MR.ASEES MOBILE 9495603778
[Quoted text hidden]

-

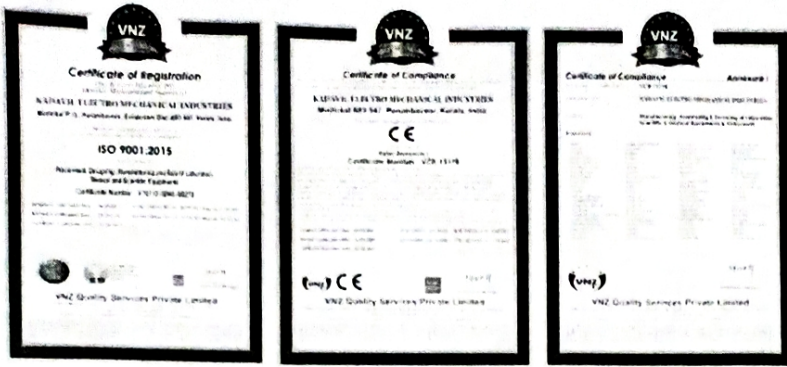


#We Supply Covid-19 Lab Equipment#

BIOLOGICAL SAFETY CABINET (CLASS-II) & (CLASS-III) # LAMINAR AIR FLOW CABINET # AUTOCLAVES # DEEP FREEZERS # CENTRIFUGES # COVID WISK # etc....

=====

M.A.Moideen,
Marketing Manager,
Kadavil Electro Mechanical Industries (KEMI).
Mob: - 09388468070

Please don't Print This E-mail Unless You Really Need To.

 Image result for please don't print this email signature
"Save Tree Save Earth"

Fri, 16 Aug, 2024 at 2:28 p

neesh P P <jineeshcyrix@gmail.com>
: Anjitha T L <purchasecyrix2@gmail.com>
: Blesson Jose <zm2.klbemp@cyrix.in>, DM Sarang-KLBEMP <dm1.klbemp@cyrix.in>

Dear Anjitha,

Please arrange quotation

Thanks & Regards,

Jineesh PP
District Incharge - Kozhikode
Mob-7593847163
jineeshcyrix@gmail.com
www.cyrixhealthcare.com

Cyrix Healthcare Pvt Ltd

| 30/641 B | Pettah Jn | Poonithura | Cochin -38 | Kerala | India

CYRIX BIOMEDICAL EQUIPMENT MAINTENANCE PROGRAMME (BEMP)




TOLL FREE NO: 1800 - 425-7669

BAR CODE - (8004-890615225)

1120685



**CYRIX HEALTH CARE PVT.LTD
BEMP SERVICE PROVIDED**

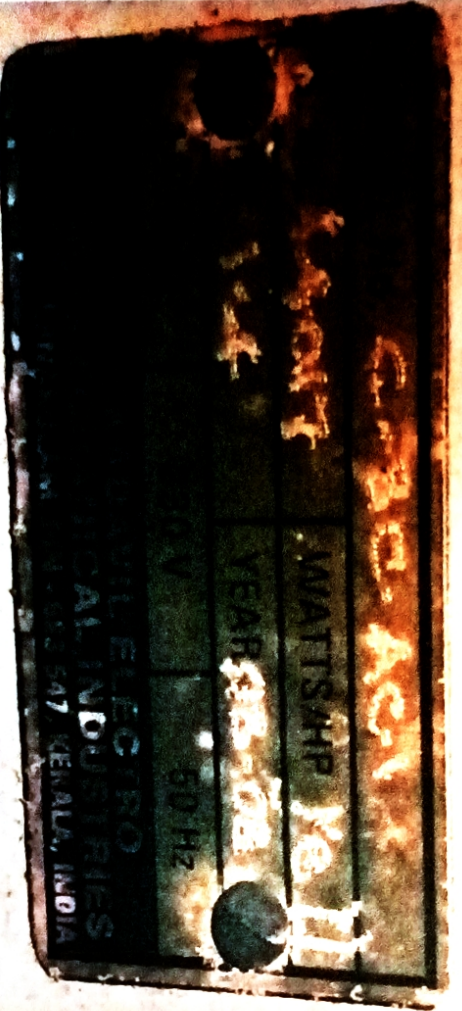

[Handwritten signature]
2/19/2011

**SUPERINTENDENT
TALUK HOSPITAL
KUTTIADY**

